Supplementary Information

Preliminary evaluation of typed decision models in mental health using motivational interviewing coding

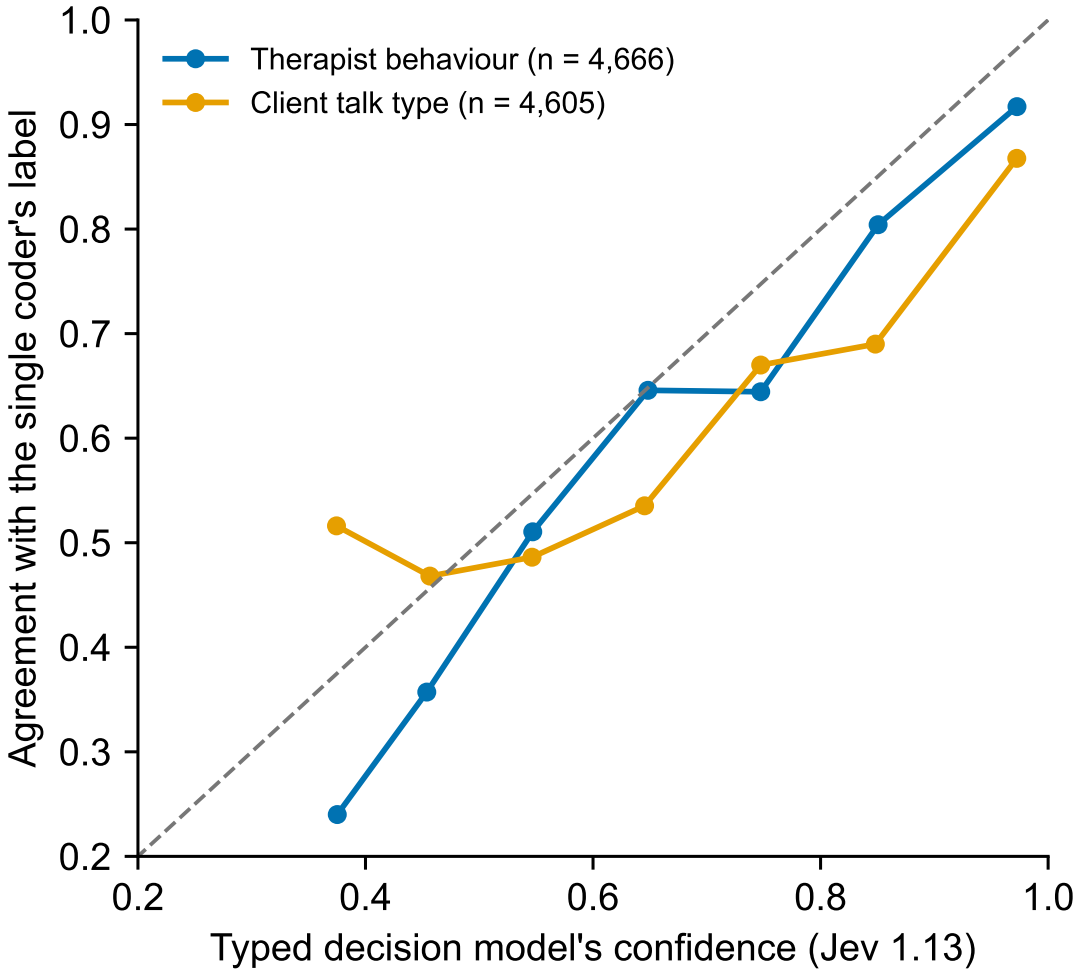

Supplementary Figure 1. Calibration against single-expert codes. The reliability diagram shows the confidence of Jev 1.13 in its selected label against agreement with the published expert code on the single-expert transcripts of AnnoMI, separately for therapist behaviour and client talk type. Confidence is divided into ten equal-width bins from 0 to 1; only bins containing at least 20 utterances are plotted. Each point shows the mean confidence and proportion of matching codes within a bin. The dashed line indicates equality between confidence and agreement. Connecting lines aid visual inspection. This descriptive diagram uses ten bins; the expected calibration error reported in the main manuscript uses the four bins specified in Methods.