


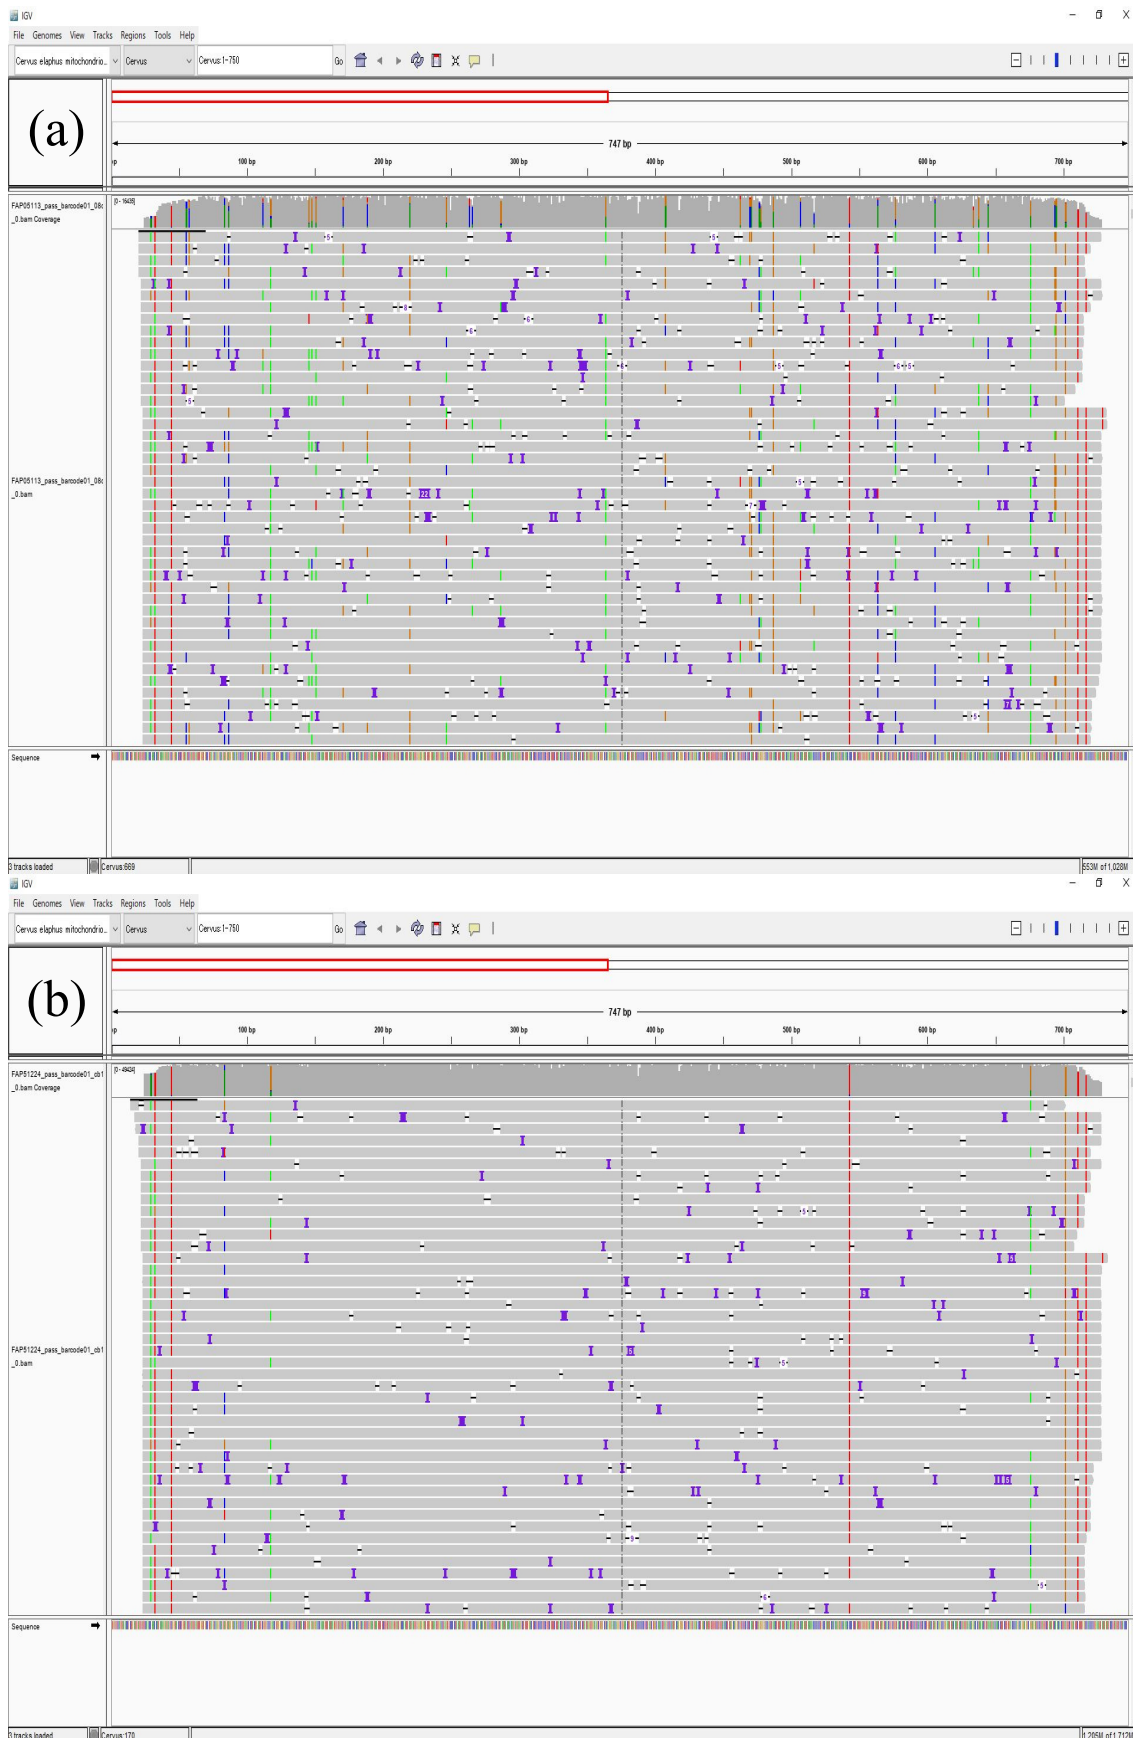

Supplemental Figure 1. Difference in base-call accuracy between Fast (a) and High-accuracy (b) modes after visualization with IGV.