


A

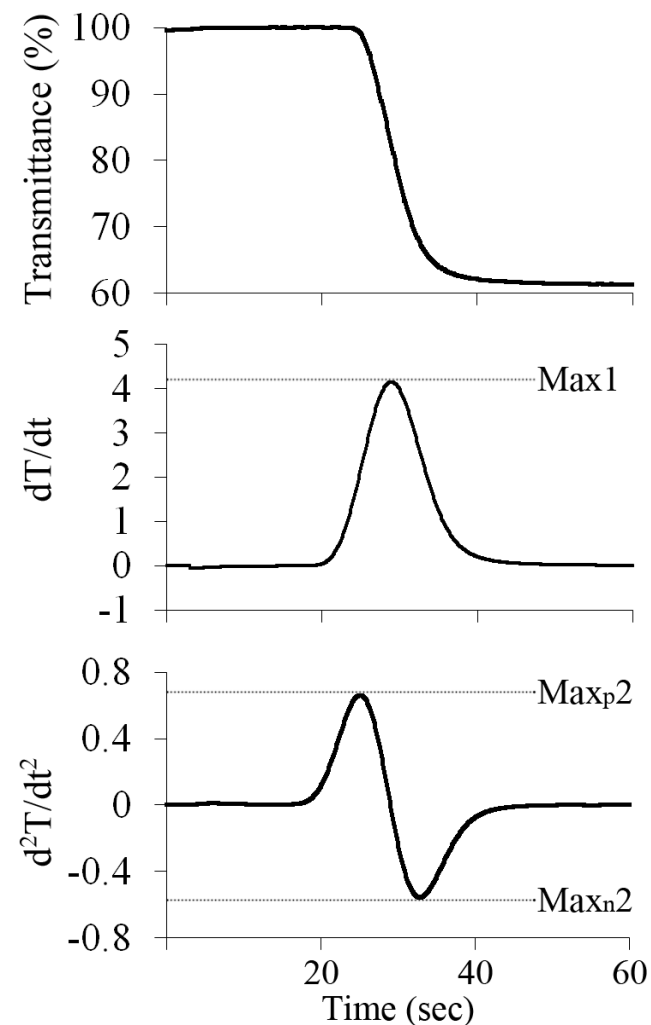

B

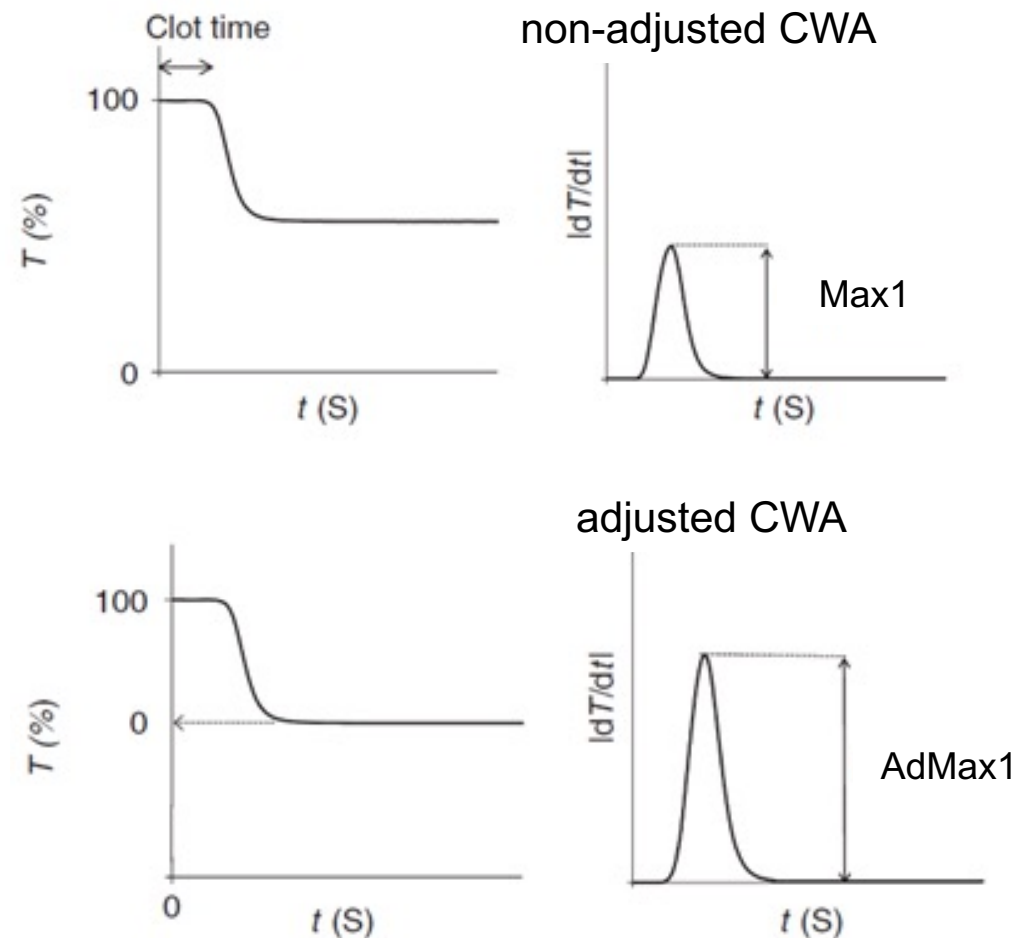


Fig. S1 A The representative explanation figure about clot waveform analysis (CWA) performed by using the automated coagulation system, CN-6000 (Sysmex). B The representative explanation figure about how to adjust CWA parameters by normalizing transmittance changes. T , transmittance; t , time; $AdMax1$, adjusted $Max1$