


1

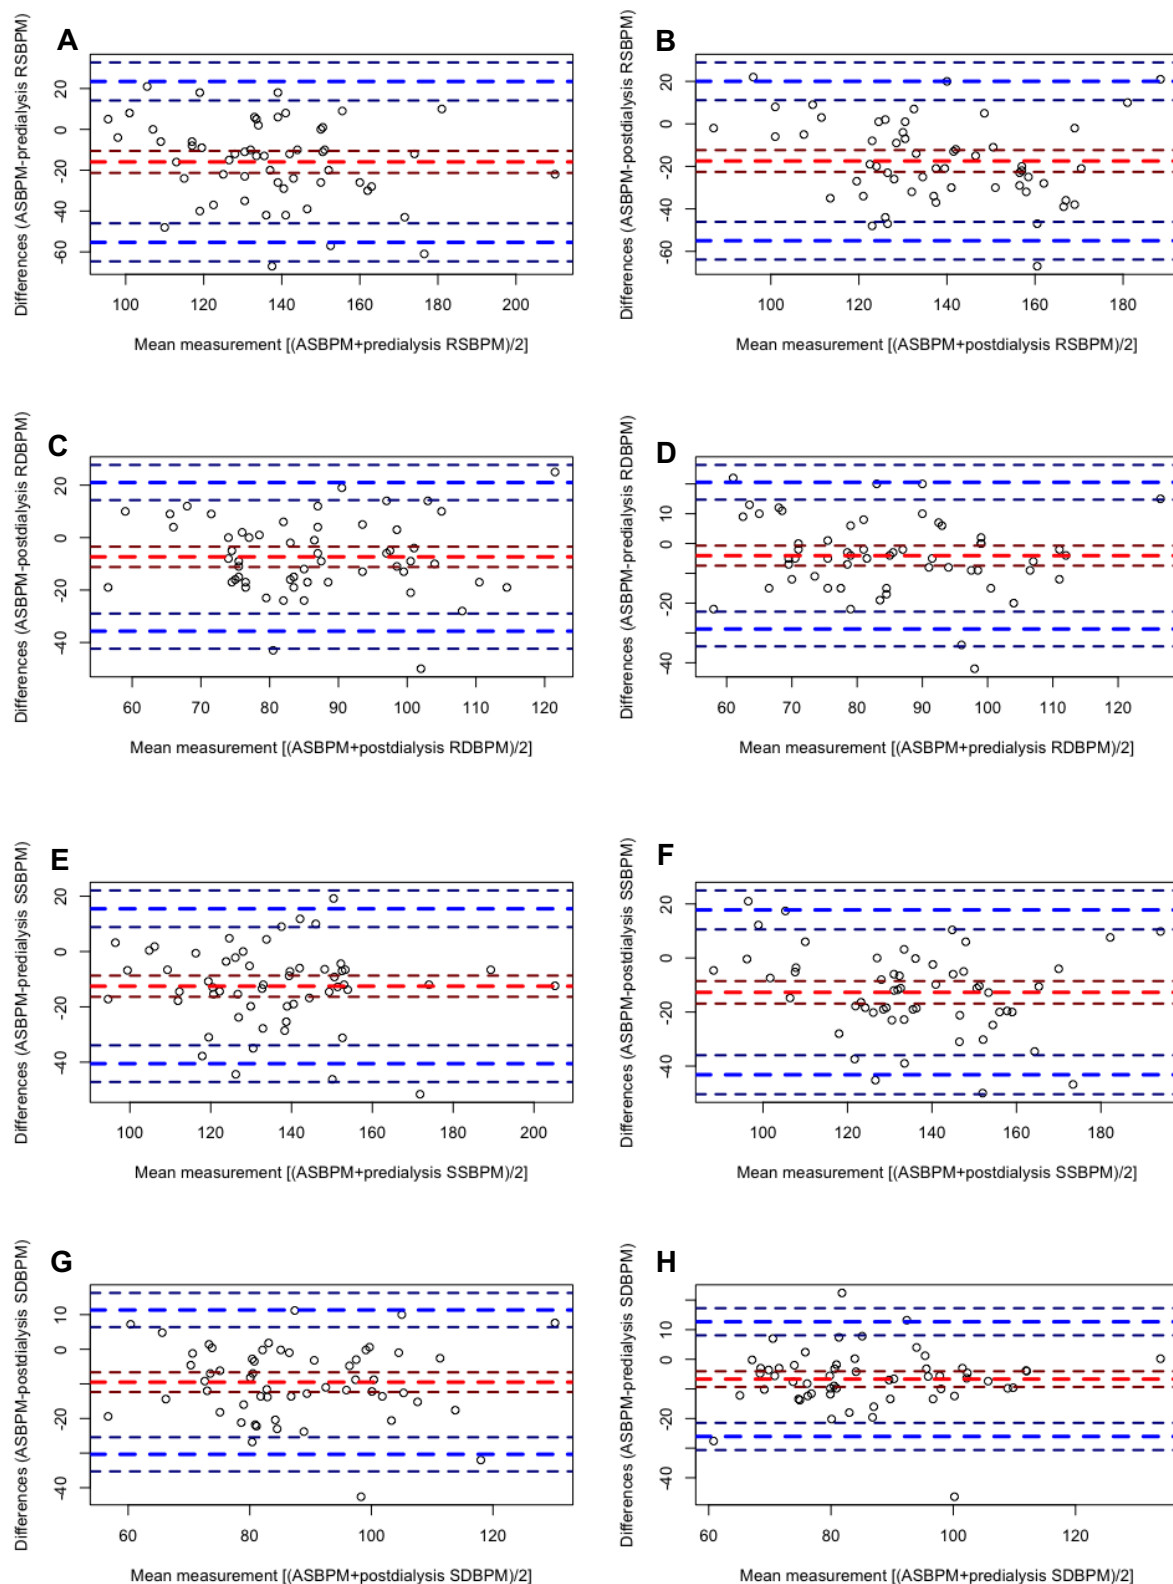

2

3

4 **Supplemental figure 1:** Agreement between hemodialysis center and ambulatory blood
 5 pressure monitoring (Bland and Altman diagram). Blood pressures obtained with routine BP

6 measurement as well as with Standardized BP measurement did not agree with blood
7 pressures obtained with the ambulatory BP monitoring. Standardized blood pressure
8 measurements in pre- and post-dialysis were significantly different from ambulatory blood
9 pressure monitoring (**A, B, C, and D**). Routine blood pressure measurements in pre- and post-
10 dialysis were significantly different from ambulatory blood pressure monitoring (**E, F, G, and**
11 **H**). Abbreviations: SSBPM, standardized systolic blood pressure measurement; RSBPM,
12 routine systolic blood pressure measurement; SDBPM, standardized diastolic blood pressure
13 measurement; RDBPM, routine diastolic blood pressure measurement.