


Supplementary Fig. 1

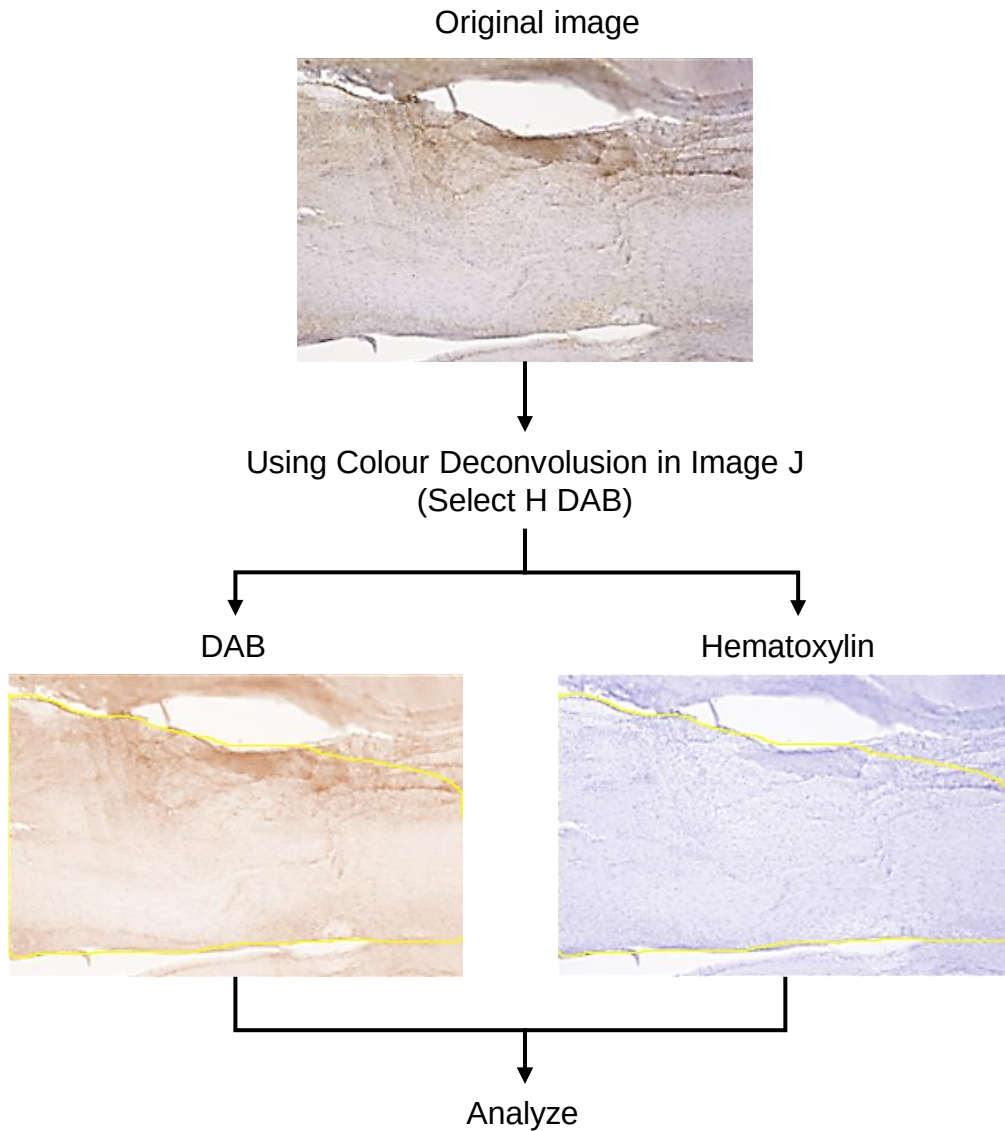

Supplementary Fig.1. Measurement of DAB% area relative to hematoxylin %area.

The original images were separated into DAB and hematoxylin by Colour Deconvolution in Image J and the %area of each was determined.