

Initial non-invasive in vivo sensing of the lung using time domain diffuse optics

Antonio Pifferi^{1,2}, Massimo Miniati³, Andrea Farina², Sanathana Konugolu Venkata Sekar⁴, Pranav Lanka⁴, Alberto Dalla Mora¹, Giulia Maffei^{1,*}, and Paola Taroni^{1,2}

¹Politecnico di Milano, Dipartimento di Fisica, 20133, Milan, Italy

²INFN-CNR, Consiglio Nazionale delle Ricerche, Istituto di Fotonica e Nanotecnologie, 20133, Milan, Italy

³University of Florence, Department of Experimental and Clinical Medicine, 50134, Florence, Italy

⁴Biophotonics@Tyndall, IPIC, Tyndall National Institute, T12R5CP, Cork, Ireland

*giulia.maffei@polimi.it

Supplementary information

The following figures are attached as supplementary figures to the main figures, showing the other protocol (Prot5) with 5s duration of each phase and 10 repetitions (the first one with normal breathing), and the non-refolded analysis.

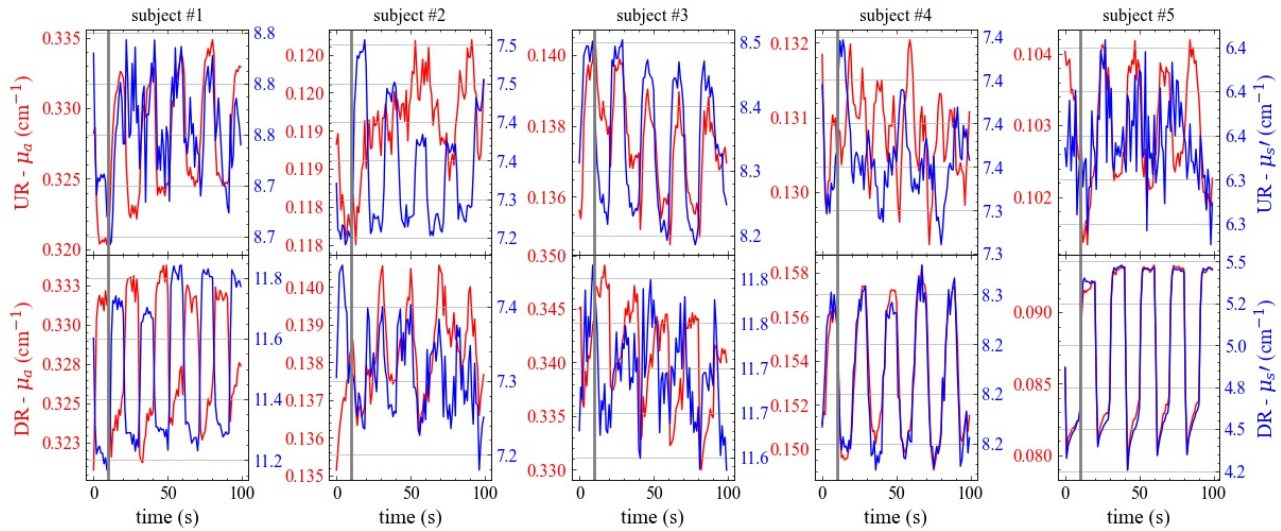


Figure 1. Supplementary Figure S1 to Fig. 5.

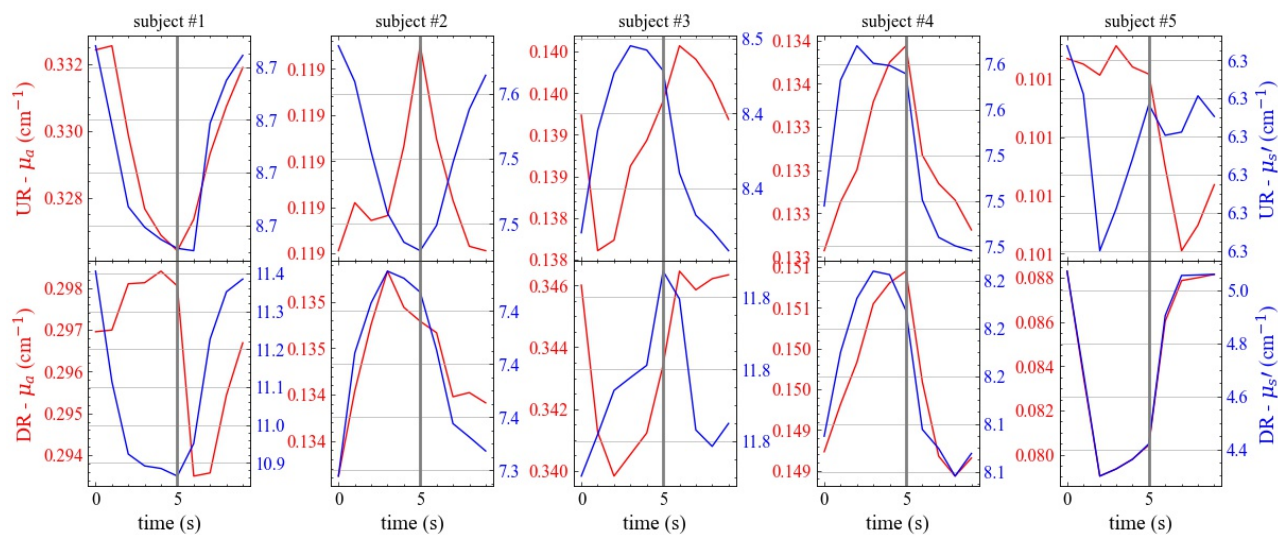


Figure 2. Supplementary Figure S2 to Fig. 5.

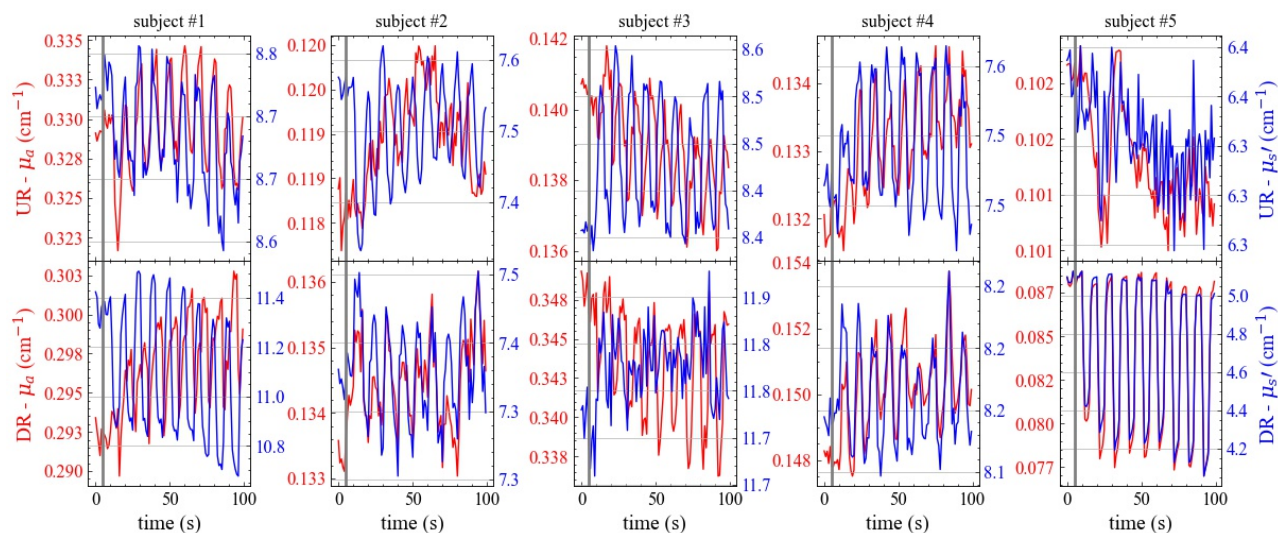


Figure 3. Supplementary Figure S3 to Fig. 5

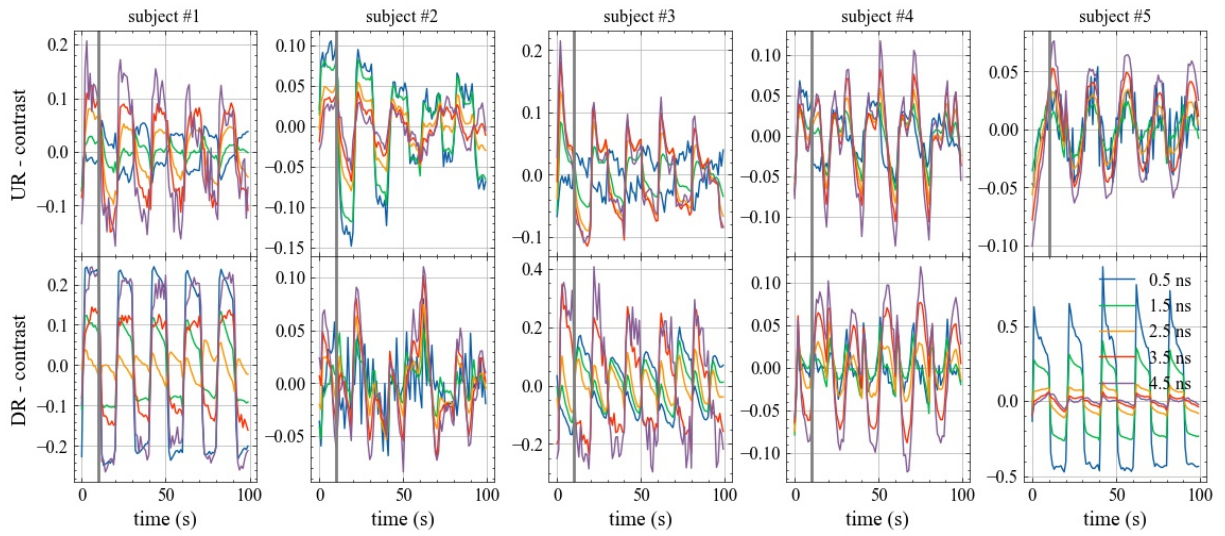


Figure 4. Supplementary Figure S4 to Fig. 6.

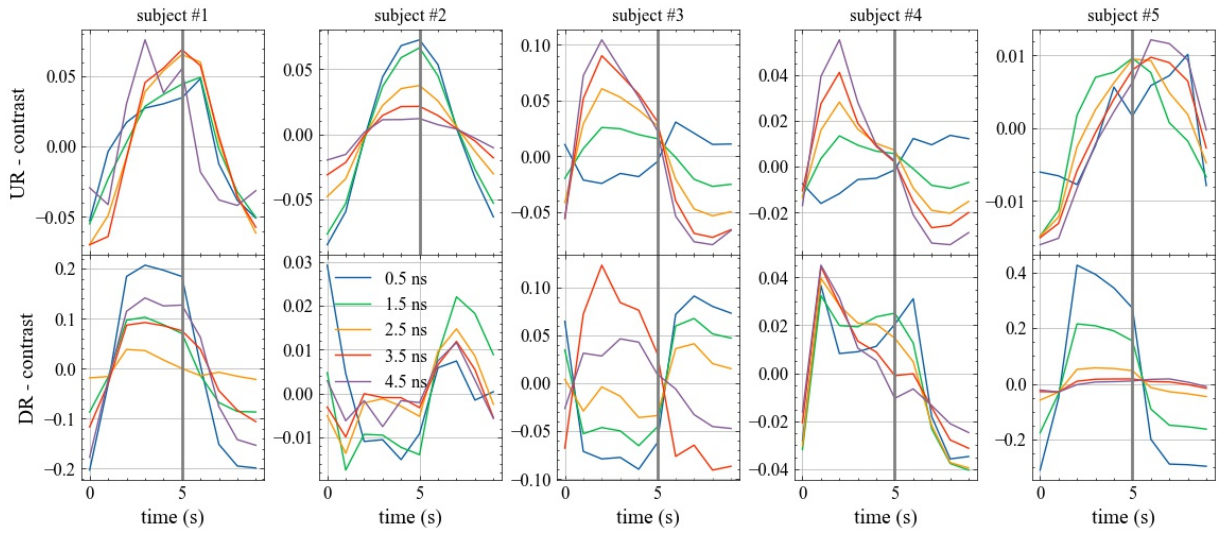


Figure 5. Supplementary Figure S5 to Fig. 6.

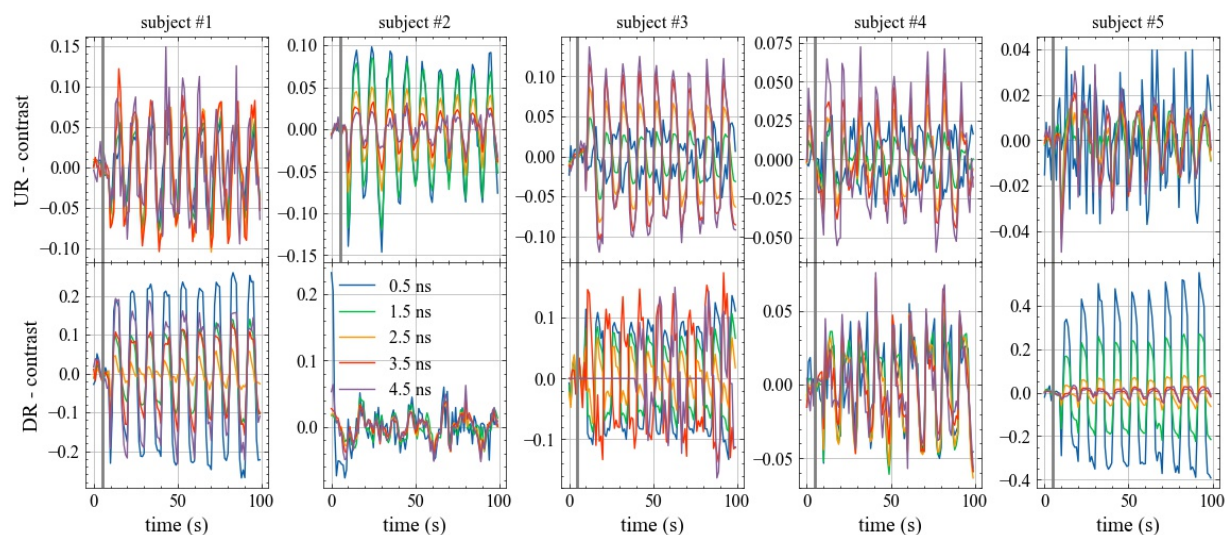


Figure 6. Supplementary Figure S6 to Fig. 6.

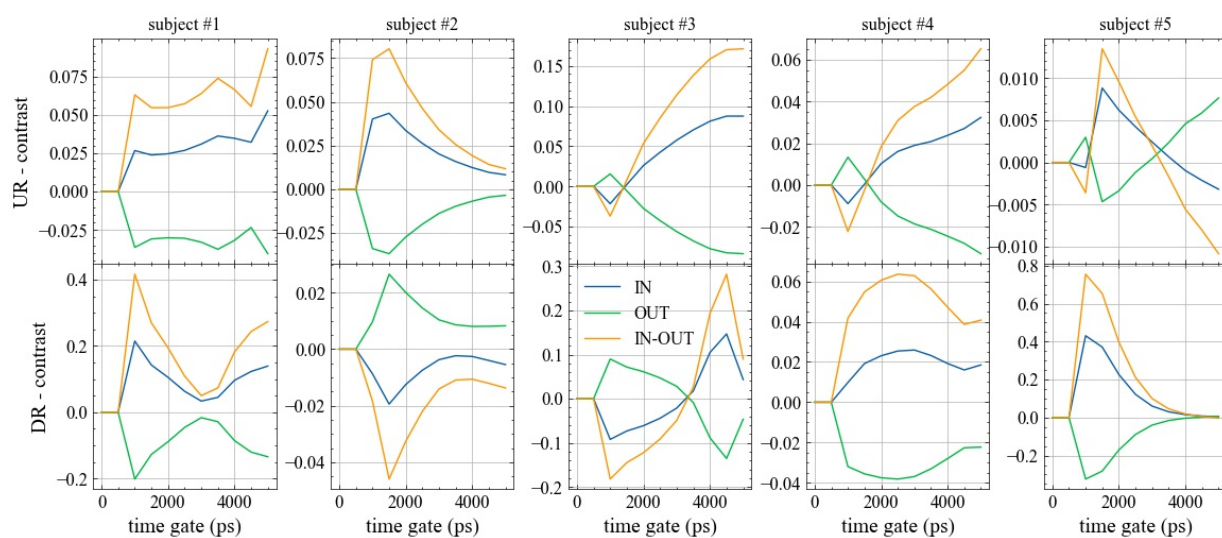


Figure 7. Supplementary Figure S7 to Fig. 7.