

Instrument Name:SA/AD/INS/015

SPARK ANALYTICAL

vial position :2


UNKNOWN PRODUCT-2

20-Sep-2024 19:17:50

SAMPLE-2-12 (0.380) Cm (5:29)

1 : Scan ES+

1.48e5

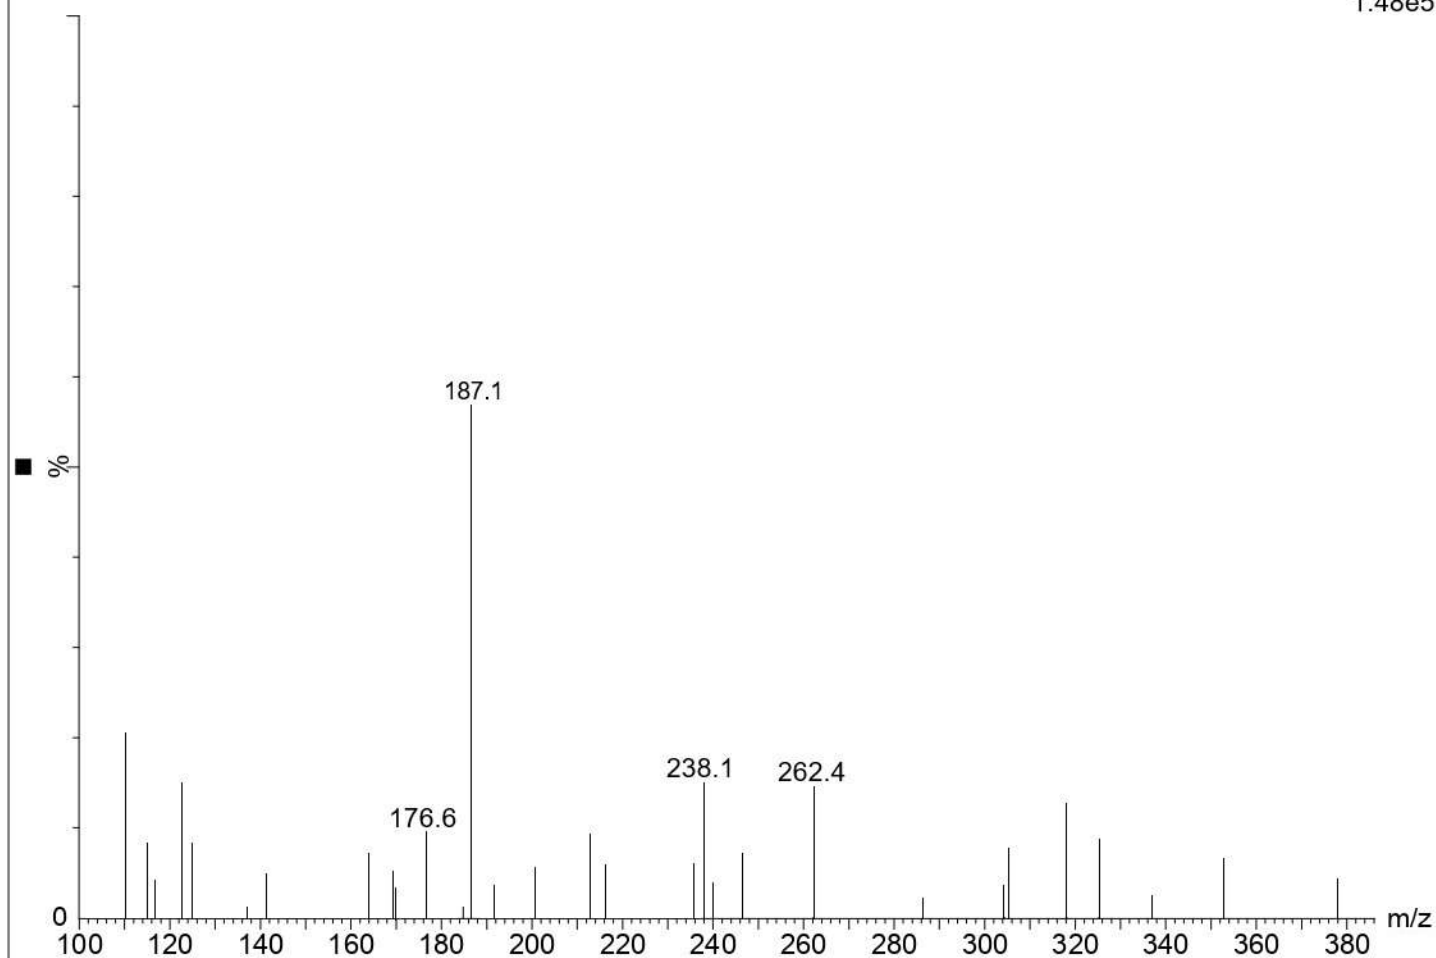

SAMPLE-2-12 (0.359) Cm (7:23)

3 : Scan ES-

2.78e3

