



## Supplementary Information

### Tables:

- Supplementary Table 1: Bills Summary.
- Supplementary Table 2: Components of the platform.
- Supplementary Table 3: Comprehensive Metabolic Panel.
- Supplementary Table 4: Statistical comparison of metabolite differences between our life support platform and standard tissue culture conditions.
- Supplementary Table 5: Organoid measures batch 1.
- Supplementary Table 6: Organoid measures batch 2.
- Supplementary Table 7: Organoid measures batch 3.
- Supplementary Table 8: Organoid normalized measures.
- Supplementary Table 9: ANOVA analysis for cross-sectional area measurements.
- Supplementary Table 10: Calibration curve at 0.52 W/mm<sup>2</sup> power intensity.
- Supplementary Table 11: Calibration curve at 0.79 W/mm<sup>2</sup> power intensity.
- Supplementary Table 12: CFD initial conditions.

### Figures:

- Supplementary Figure 1: Resolution and Field of View (FOV) Assessment.
- Supplementary Figure 2: PDMS/Glass chip multiwell configuration.
- Supplementary Figure 3: Experimental design of the fluid flow characterization.
- Supplementary Figure 4: Viability of cortical organoids grown in the life support platform.
- Supplementary Figure 5: Viability of cortical organoids grown in a standard tissue culture incubator.
- Supplementary Figure 6: Viability of cortical organoids grown in the life support platform for well 3 of the multiwell approach.
- Supplementary Figure 7: Longitudinal growth of cortical organoid in batch 1.
- Supplementary Figure 8: Longitudinal growth of cortical organoid in batch 2.
- Supplementary Figure 9: Longitudinal growth of cortical organoid in batch 3.

Supplementary Table 1: Bills Summary

Component	Unit	Unit Cost (USD)	Subtotal	Source of Material	Model type/Material
Arduino Mega 2560 R3	1	\$48.40	\$48.40	<a href="https://www.sparkfun.com/products/11061">https://www.sparkfun.com/products/11061</a>	DEV-11061 RoHS
CD-40CO2/Temperature /Humidity Sensor	1	\$44.95	\$44.95	<a href="https://www.adafruit.com/product/5187">https://www.adafruit.com/product/5187</a>	STEMMA QT / Qwiic
FeatherS2 - ESP32	1	\$24.95	\$24.95	<a href="https://www.adafruit.com/product/4769">https://www.adafruit.com/product/4769</a>	S2
Cavro Centris Pump	1	\$5,000	\$5,000	<a href="https://partnering.tecan.com/cavro-centris-pump-for-oem-liquid-handling">https://partnering.tecan.com/cavro-centris-pump-for-oem-liquid-handling</a>	Cavro
PTC Heating Element AC DC 12V Aluminum Shell	1	\$7.51	\$7.51	<a href="https://www.amazon.com/Aluminum-Temperature-Thermostatic-Applicable-Minature/dp/B07GBNGB4L/">https://www.amazon.com/Aluminum-Temperature-Thermostatic-Applicable-Minature/dp/B07GBNGB4L/</a>	Aluminum
Uxcell 10K NTC Thermistor Probe	1	\$8.49	\$8.49	<a href="https://www.amazon.com/uxcell-Thermistor-Sensitive-Temperature-Conditioner/dp/B07LGLCYFP?th=1">https://www.amazon.com/uxcell-Thermistor-Sensitive-Temperature-Conditioner/dp/B07LGLCYFP?th=1</a>	Epoxy
W1209 12V DC Digital Temperature Controller	1	\$8.49	\$8.49	<a href="https://www.amazon.com/HiLetgo-Temperature-Controller-Thermostat-One-Channel/dp/B07CH7W3XP?th=1">https://www.amazon.com/HiLetgo-Temperature-Controller-Thermostat-One-Channel/dp/B07CH7W3XP?th=1</a>	B07CH7W3XP
Dino-Lite Edge	1	\$899.00	\$899.00	<a href="https://www.auroraprosci.com/Digital-Microscope-AM4115T-GRFBY">https://www.auroraprosci.com/Digital-Microscope-AM4115T-GRFBY</a>	AM4115TGRFBY
ALITOVE 12V 5A 60W Power Supply Adapter	1	\$12.99	\$12.99	<a href="https://www.amazon.com/dp/B078RY6YY3">https://www.amazon.com/dp/B078RY6YY3</a>	AL12V5AT
100ml Thick Glass Media Storage	1	\$6.99	\$6.99	<a href="https://www.amazon.com/Storage-Bottles-Graduations-Scientific-Containers/dp/B07Y65GN1S/">https://www.amazon.com/Storage-Bottles-Graduations-Scientific-Containers/dp/B07Y65GN1S/</a>	CQ15707
TAILONZ PNEUMATIC 1/4 Inch NPT 12V/24V/110V/220V	1	\$17.99	\$17.99	<a href="https://www.amazon.com/Tailonz-Pneumatic-Electric-Solenoid-2W025-08/dp/B07X287BSX/?th=1">https://www.amazon.com/Tailonz-Pneumatic-Electric-Solenoid-2W025-08/dp/B07X287BSX/?th=1</a>	2W025-08
Raspberry Pi 4 Model B	1	\$77.99	\$77.99	<a href="https://www.amazon.com/Raspberry-Model-2019-Quad-Bluetooth/dp/B07TC2BK1X/">https://www.amazon.com/Raspberry-Model-2019-Quad-Bluetooth/dp/B07TC2BK1X/</a>	RAS-4-4G
ELECROW 5 Inch Raspberry Pi Screen Touchscreen	1	\$43.99	\$43.99	<a href="https://www.amazon.com/Elecrow-800x480-Interface-Supports-Raspberry/dp/B013JECYF2/">https://www.amazon.com/Elecrow-800x480-Interface-Supports-Raspberry/dp/B013JECYF2/</a>	ILI9486L
ph Kit Atlas Scientific	1	\$149.00	\$149.00	<a href="https://atlas-scientific.com/kits/ph-kit/">https://atlas-scientific.com/kits/ph-kit/</a>	#KIT-101P
Mini Lab Grade pH Probe	1	\$60.99	\$60.99	<a href="https://atlas-scientific.com/probes/miniphprobe/">https://atlas-scientific.com/probes/miniphprobe/</a>	#ENV-20-pH
SYLGARD™ 184 Silicone Elastomer Kit	1	\$154	\$154	<a href="https://kayden.com/productdetail/dc4019862/dc-184-sylgard-05kg-11lb-kit">https://kayden.com/productdetail/dc4019862/dc-184-sylgard-05kg-11lb-kit</a>	Silicone
Plus Microscope Slides	1	\$211.50	\$211.50	<a href="https://www.fishersci.com/shop/products/fisherbrand-superfrost-plus-microscope-slides-2/1255015">https://www.fishersci.com/shop/products/fisherbrand-superfrost-plus-microscope-slides-2/1255015</a>	Glass
Model Resin Formlabs	1	\$149	\$149	<a href="https://dental.formlabs.com/store/materials/model-resin/">https://dental.formlabs.com/store/materials/model-resin/</a>	Resin

CO2 Stainless Steel Diffuser	1	\$15.99	\$15.99	<a href="https://www.amazon.com/YOU-Stainless-Diffuser-Regulator-Freshwater/">https://www.amazon.com/YOU-Stainless-Diffuser-Regulator-Freshwater/</a>	Stainless Steel
NeoPixel Ring	1	\$16.95	\$16.95	<a href="https://www.adafruit.com/product/1586/">https://www.adafruit.com/product/1586/</a>	5050 RGB LED
Adjustable Precision Mount	1	\$199.00	\$199.00	<a href="https://www.dinolite.us/products/accessories">https://www.dinolite.us/products/accessories</a>	Stainless Steel
Polyvinylidene Fluoride (PVDF) Filter	1	\$2.69	\$2.69	<a href="https://www.perkinelmer.com/product/filterpvdf-syringe-25mm-22um-pk-100-02542918">https://www.perkinelmer.com/product/filterpvdf-syringe-25mm-22um-pk-100-02542918</a>	Polyvinylidene fluoride

Supplementary Table 2: Components of the platform

Number	Descriptor	Repository
1	Arduino mega pH Solenoid.ino	braingeneersdifussionproject/Arduino/
2	ImageProcessing.m	braingeneersdifussionproject/MATLAB/
3	ObtainVideoFrames.m	braingeneersdifussionproject/MATLAB/
4	ObtainVideoFrames V2.m	braingeneersdifussionproject/MATLAB/
5	ReduceVideoSize.m	braingeneersdifussionproject/MATLAB/
6	CO2TempHumidityRecording.py	braingeneersdifussionproject/Python/Enviroment_Sensor/
7	MainPumpProgramExe.py	braingeneersdifussionproject/Python/Servo_Pump/Apps/
8	PDMS Mold V1.stl	braingeneersdifussionproject/Print_Files/
9	Hole Base.stl	braingeneersdifussionproject/Print_Files/
10	BioChamber Base.stl	braingeneersdifussionproject/Print_Files/
11	Cap Biochamber.stl	braingeneersdifussionproject/Print_Files/
12	EnviromentalSensor BaseCase.stl	braingeneersdifussionproject/Print_Files/
13	EnviromentalSensor TopCase.stl	braingeneersdifussionproject/Print_Files/
14	GFP Chamber.stl	braingeneersdifussionproject/Print_Files/
15	GFP Chamber Cap.stl	braingeneersdifussionproject/Print_Files/
16	Heater Holder.stl	braingeneersdifussionproject/Print_Files/
17	Heater Holder Biochamber.stl	braingeneersdifussionproject/Print_Files/
18	Holder Biochamber Left.stl	braingeneersdifussionproject/Print_Files/
19	Holder Biochamber Rigth.stl	braingeneersdifussionproject/Print_Files/
20	Microscope Holder.stl	braingeneersdifussionproject/Print_Files/
21	Pump Holder .stl	braingeneersdifussionproject/Print_Files/
22	RaspberryPi Holder.stl	braingeneersdifussionproject/Print_Files/
23	ReservoirCap Left.stl	braingeneersdifussionproject/Print_Files/
24	ReservoirCap Rigth.stl	braingeneersdifussionproject/Print_Files/
25	SourcePower Holder.stl	braingeneersdifussionproject/Print_Files/
26	pHController Botom.stl	braingeneersdifussionproject/Print_Files/
27	pHController Top.stl	braingeneersdifussionproject/Print_Files/
28	CO2 Holder.stl	braingeneersdifussionproject/Print_Files/
29	RawData	braingeneersdifussionproject/RawData/

Supplementary Table 3. Comprehensive Metabolic Panel

Test name	Unit	Fresh Media	Platform D3			Incubator D6			Platform D6		
			B1	B2	B3	B1	B2	B3	B1	B2	B3
pH	-	7.82	7.88	7.85	7.44	7.83	7.82	7.81	7.59	7.69	7.21
cGlu	g/L	2.92	2.93	3.44	2.96	2.63	3.20	2.78	2.77	3.36	3.10
ck	mM	3.87	3.90	6.40	6.00	4.10	5.60	4.40	4.90	5.80	6.00
cNa <sup>+</sup>	mM	146.00	146.00	174.00	157.00	152.00	218.00	185.00	138.00	169.00	182.00
cCa <sup>2+</sup>	mM	0.80	0.85	0.87	0.78	0.86	1.08	0.91	0.79	0.89	0.84
cCl <sup>-</sup>	mM	123.00	125.00	149.00	129.00	130.00	184.00	141.00	119.00	144.00	135.00

Supplementary Table 4. Statistical comparison of metabolite differences between our life support platform and standard tissue culture conditions

Metabolite	Chi-Square	df	p-Value
pH	4.79	3	0.1874
cGlu	2.93	3	0.4012
cK	7.32	3	0.0623
cNa <sup>+</sup>	3.55	3	0.2073
cCa <sup>2+</sup>	5.12	3	0.1630
cCl <sup>-</sup>	4.19	3	0.1781

\*The margin of error presented here corresponds to a 95% confidence interval

Supplementary Table 5: Organoid cross-sectional measures batch 1 in mm<sup>2</sup>.

Days	PG0	PG1	PG2	PG3	Average PG	Standard Deviation
15	0.35	0.34	0.37	0.35	0.35	0.012
16	0.39	0.34	0.39	0.38	0.38	0.02
17	0.42	0.40	0.43	0.42	0.42	0.01
18	0.43	0.40	0.43	0.43	0.42	0.01
19	0.44	0.42	0.44	0.43	0.43	0.01
20	0.45	0.42	0.49	0.46	0.45	0.03

Supplementary Table 6: Organoid cross-sectional measures batch 2 in mm<sup>2</sup>.

Days	PG0	PG1	Average PG	Standard Deviation
15	2.02	2.03	0.006	2.02
16	2.26	2.06	0.146	2.16
17	2.35	2.11	0.175	2.23
18	2.48	2.11	0.264	2.29
19	2.51	2.14	0.261	2.32
20	2.71	2.28	0.304	2.50

Supplementary Table 7: Organoid cross-sectional measures batch 3 in mm<sup>2</sup>.

Days	PG0	PG1	PG2	Average PG	Standard Deviation
15	1.16	1.27	1.47	0.162	1.30
16	1.36	1.49	1.61	0.122	1.49
17	1.43	1.57	1.63	0.099	1.54
18	1.50	1.68	1.73	0.121	1.63
19	1.50	1.68	1.75	0.129	1.64
20	1.52	1.69	1.78	0.135	1.66

Supplementary Table 8: Organoid normalized measures.

Days	Z1	Z1	Z1	Z1	Z2	Z2	Z3	Z3	Z3
0	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00
1	-1.57	-3.00	4.99	-0.43	-0.22	0.22	-11.11	-2.33	13.44
2	10.70	-2.14	12.41	8.70	11.78	1.56	4.90	14.83	23.76
3	18.97	12.70	22.11	20.97	16.28	4.08	10.36	20.45	25.37
4	23.82	14.98	23.54	21.83	22.55	4.12	15.29	28.99	32.99
5	25.25	18.97	25.53	23.54	23.88	5.66	15.44	29.45	34.76
6	28.96	18.69	39.80	30.96	33.86	12.62	16.75	29.99	37.22

Supplementary Table 9: ANOVA analysis for cross-sectional area measurements.

	sum_sq	DF	F(Anova)	p(>F)
C(Batch)	0.00585120068	2	4.1635356	0.08621606872
Residual	0.003513360544	5		

Supplementary Table 10: Calibration curve at 0.52 W/mm<sup>2</sup> power intensity.

Con. (mM)	M1		M2		M3		Standard Deviation	Power Intensity Average
	Pixel Intensity	Power Intensity	Pixel Intensity	Power Intensity	Pixel Intensity	Power Intensity		
0	6.460	0.146	4.474	0.101	4.526	0.102	0.026	0.117
1	8.110	0.183	4.544	0.103	4.504	0.102	0.047	0.129
2	9.770	0.221	12.822	0.290	12.786	0.289	0.040	0.267
3	11.420	0.258	7.666	0.173	7.620	0.172	0.049	0.201
4	13.070	0.296	11.063	0.250	10.993	0.249	0.027	0.265
5	14.730	0.333	12.799	0.289	12.716	0.288	0.026	0.303
6	16.380	0.370	18.004	0.407	18.012	0.407	0.021	0.395
7	18.030	0.408	20.081	0.454	20.170	0.456	0.027	0.439
8	19.680	0.445	20.062	0.454	20.031	0.453	0.005	0.451
9	21.340	0.483	20.621	0.466	20.561	0.465	0.010	0.471
10	22.990	0.520	21.460	0.485	21.388	0.484	0.020	0.496

Supplementary Table 11: Calibration curve at 0.79 W/mm<sup>2</sup> power intensity.


Con. (mM)	M1		M2		M3		Standard Deviation	Power Intensity Average
	Pixel Intensity	Power Intensity	Pixel Intensity	Power Intensity	Pixel Intensity	Power Intensity		
0	8.913	0.147	8.389	0.139	8.861	0.147	0.005	0.144
1	12.798	0.212	10.178	0.168	9.413	0.156	0.029	0.179
2	16.683	0.276	13.115	0.217	14.011	0.232	0.031	0.242
3	20.568	0.340	20.651	0.342	20.510	0.339	0.001	0.340
4	24.453	0.404	24.227	0.401	23.251	0.385	0.011	0.397
5	28.337	0.469	30.524	0.505	30.891	0.511	0.023	0.495

<b>6</b>	32.222	0.533	36.171	0.598	36.663	0.606	0.040	0.579
<b>7</b>	36.107	0.597	37.482	0.620	37.538	0.621	0.013	0.613
<b>8</b>	39.992	0.661	42.667	0.706	43.418	0.718	0.030	0.695
<b>9</b>	43.877	0.726	40.388	0.668	40.023	0.662	0.035	0.685
<b>10</b>	47.762	0.790	47.361	0.783	47.865	0.792	0.004	0.788


Supplementary Table 12. CFD Initial Conditions.

Variable	Value	Units
<b>Inlet-Outlet Initial Velocities</b>	0.02	m/s
<b>Diffusion Coefficient<sup>[11]</sup></b>	1.00x10 <sup>-10</sup>	m <sup>2</sup> /s
<b>Initial Concentration</b>	10	mol/m <sup>3</sup>
<b>Density</b>	1000	kg/m <sup>3</sup>
<b>Dynamic Viscosity</b>	0.002-0.003	Pa.s
<b>Porosity</b>	0.15	a.u.
<b>Number of elements</b>	519.830	Elements


USAF 1951 resolution test target

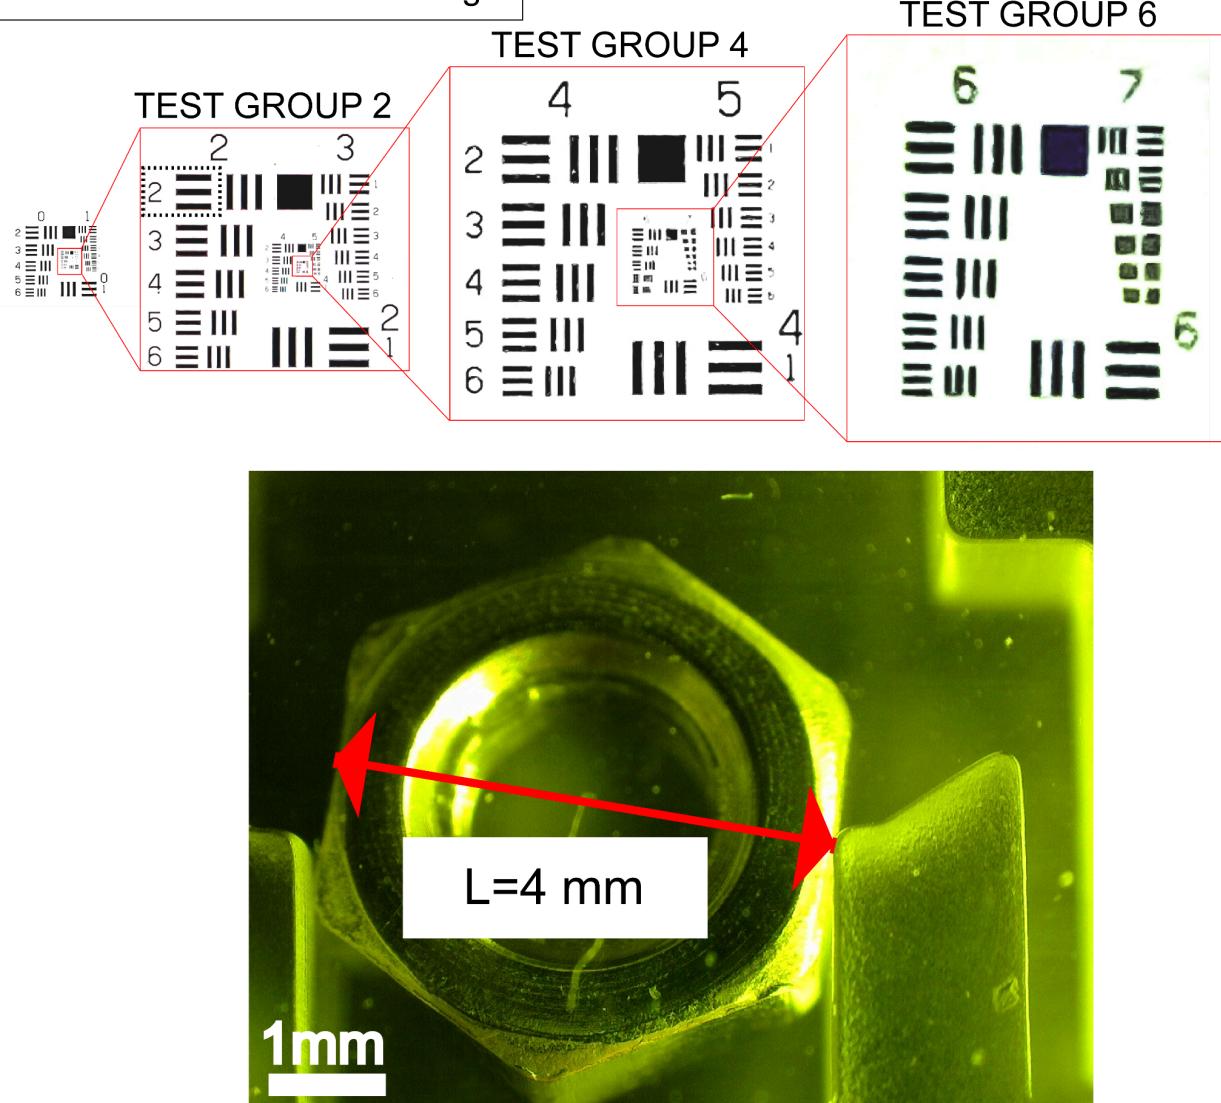


Supplementary Figure 1. Resolution and Field of View (FOV) Assessment. To assess the imaging resolution, a USAF 1951 resolution test target was used. Based on the captured images, the system resolved features up to Group 2, Element 2 (black dotted square), corresponding to 4.00 line pairs per millimeter (lp/mm), or approximately 4 mm resolution. The image below illustrates the total field of view (FOV), with the central region highlighted—this area was used for resolution analysis.

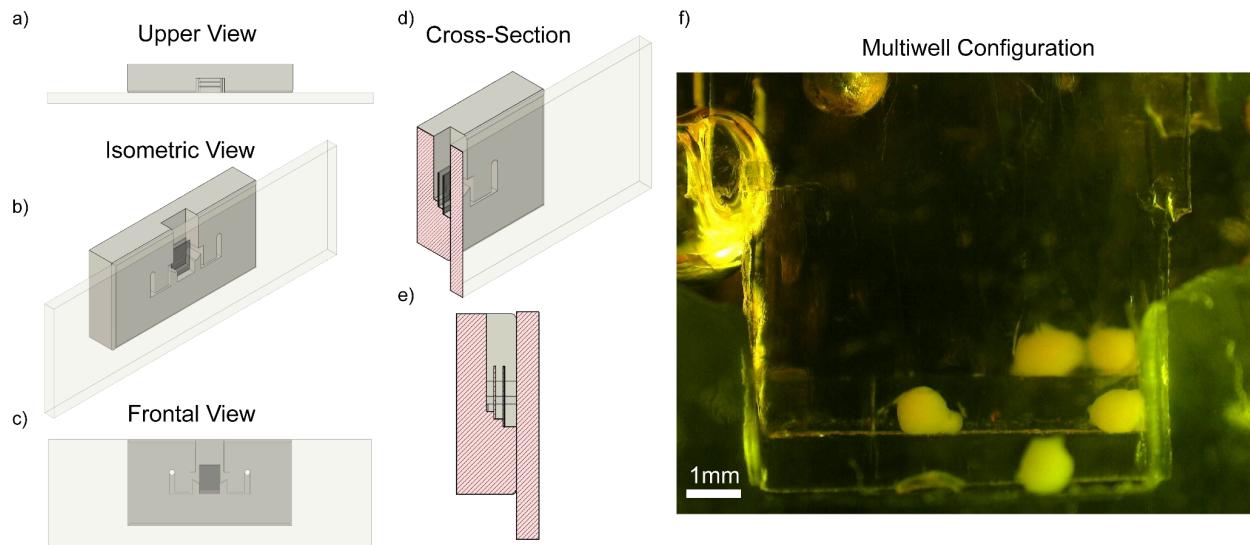


Supplementary Figure 2. Multiwell PDMS/Glass chip design and experimental validation for 3D organoid culture. **(a–e)** Design schematics of the multi-layer PDMS-glass microfluidic device. **a)** Side view showing chamber depth and channel arrangement. **b)** Transparent 3D overview highlighting the central chamber and side channels. **c)** Sectional 3D cutaway revealing vertical geometry and inlet-outlet positioning for media circulation. **d)** Detailed vertical cross-section through the chamber, indicating the stair-stepped architecture for organoid trapping and media perfusion. **e)** Top-down view of the whole device layout, displaying inlet ports and chamber configuration. **f)** Bright field image of the fabricated microfluidic chip seeded with cerebral organoids. The chamber contains multiple trapped organoids arranged along the stepped geometry. The 1 mm scale bar confirms chamber compatibility with tissue sizes in the range of  $\sim 500\text{--}800\text{ }\mu\text{m}$ , enabling confined long-term culture under continuous flow conditions.

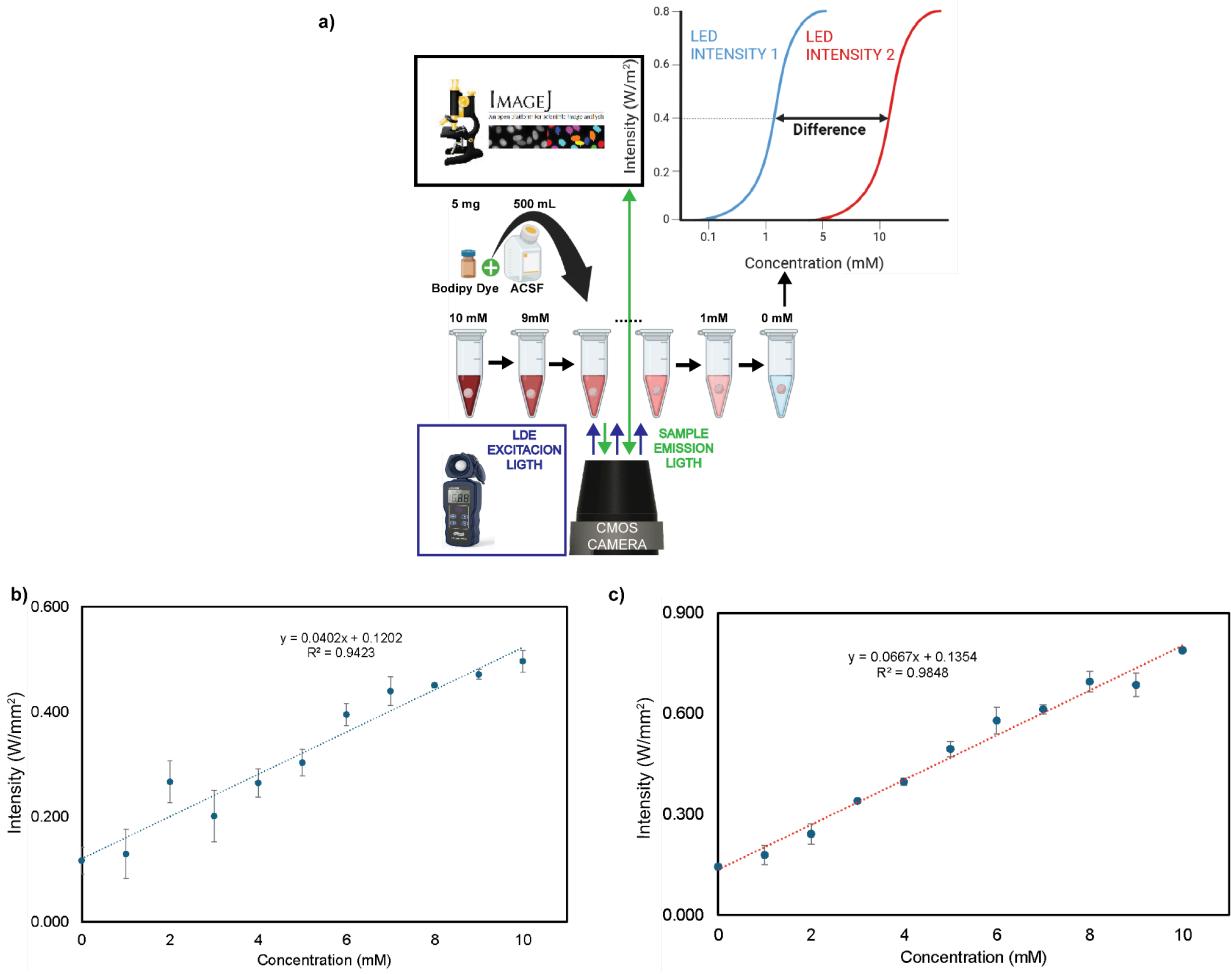


Supplementary Figure 3. illustrates the calibration and recording procedure for absorbing the green Bodipy dye. Panel **a)** The green BODIPY dye was diluted in ACSF medium to achieve concentrations ranging from 0 to 10 mM. The dye was then imaged using the AM4115T-GRFBY Dinolite, which provides camera capture and light source generation capabilities. The light intensity was measured in lux (LX) using a LX1332B light meter corresponding to the blue square. The microscope could switch between six intensity levels, with the two highest levels selected for constructing the calibration curves. ImageJ measured the intensity levels from the microscope camera, corresponding to the black square. LX was converted to lumens and power intensity (W/mm<sup>2</sup>). The calibration curve was generated using ten concentration points and replicated thrice. Panel **b)** shows the calibration curve for the 0.52 W/mm<sup>2</sup> value, corresponding to the second-highest intensity. Panel **c)** shows the highest intensity of 0.79 W/mm<sup>2</sup>. Other intensity points were not considered due to their lack of emission. The process of concentration intensity calibration for the highest intensities is shown in supplementary tables 8 and 9, respectively. Figure 3a was produced in Biorender, Image J, photograph taken by the authors, and edited in Adobe Illustrator.

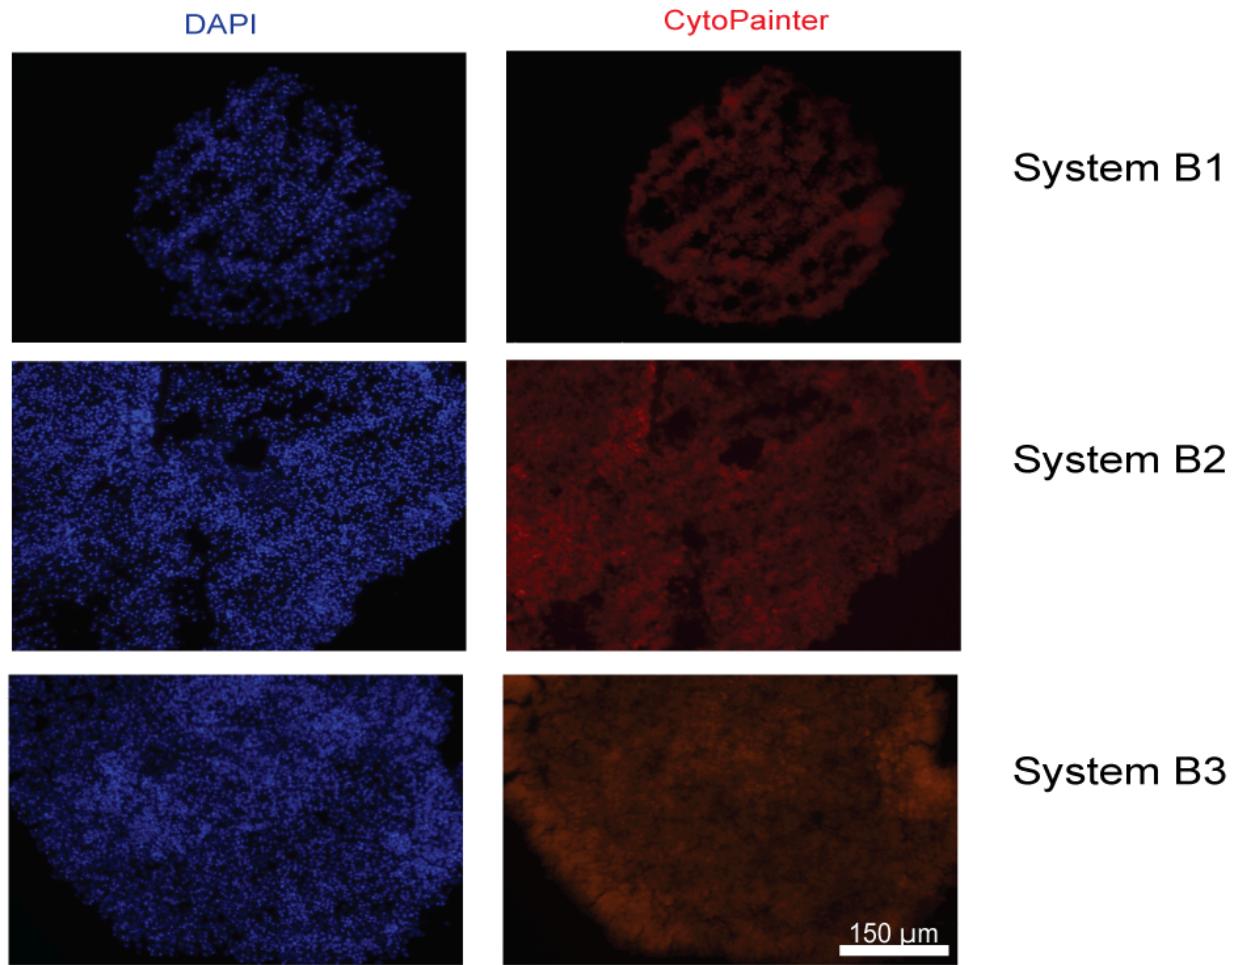

Supplementary Figure 4. Viability of cortical organoids grown in our life support platform. Representative images of D20 cortical organoids stained with CytoPainter after 120 hours are on our life support platform. A representative image from the three batches (b) analyzed is shown.

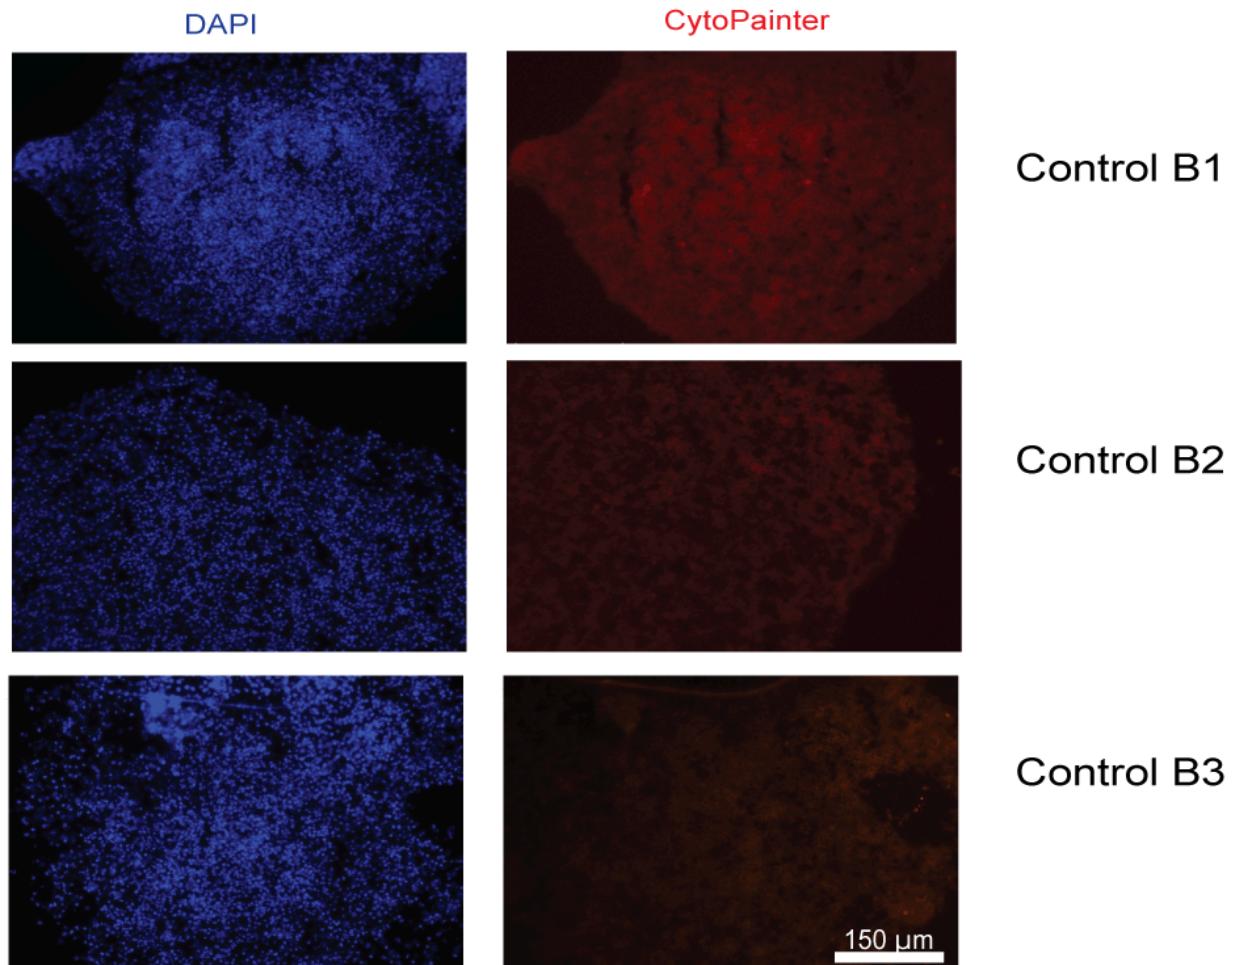


Supplementary Figure 5. Viability of cortical organoids grown in a standard tissue culture incubator. Representative images of D20 cortical organoids stained with CytoPainter. Organoids were grown in standard tissue culture conditions. A representative image from the three batches (b) analyzed is shown.

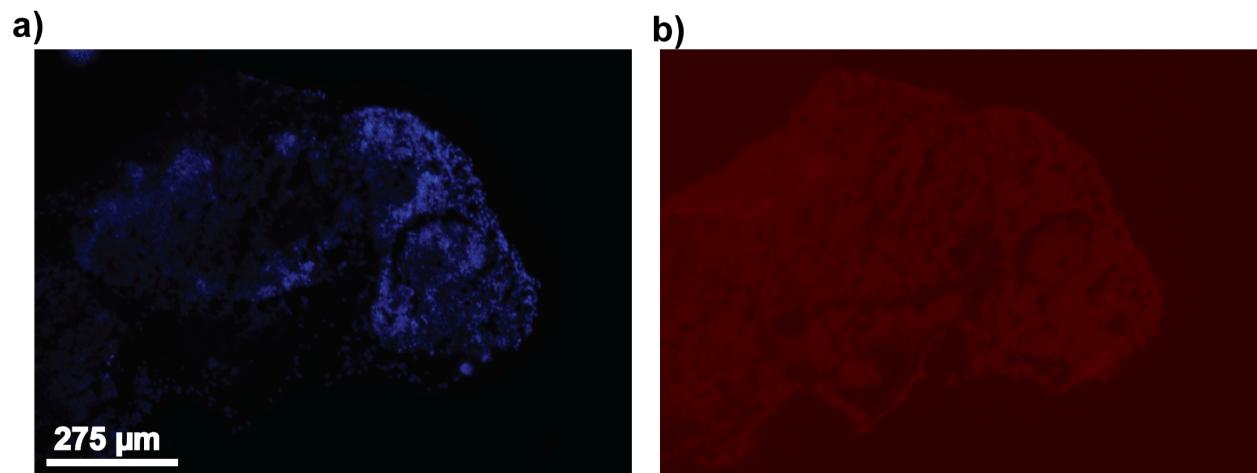


Supplementary Figure 6. Viability of cortical organoids grown in a standard tissue culture incubator. Representative images of D20 cortical organoids stained with CytoPainter. Organoids were grown in standard tissue culture conditions. A representative image from well 3 in the multiwell chip approach, (a) staining in DAPI, and (b) stained with CytoPainter.


a)

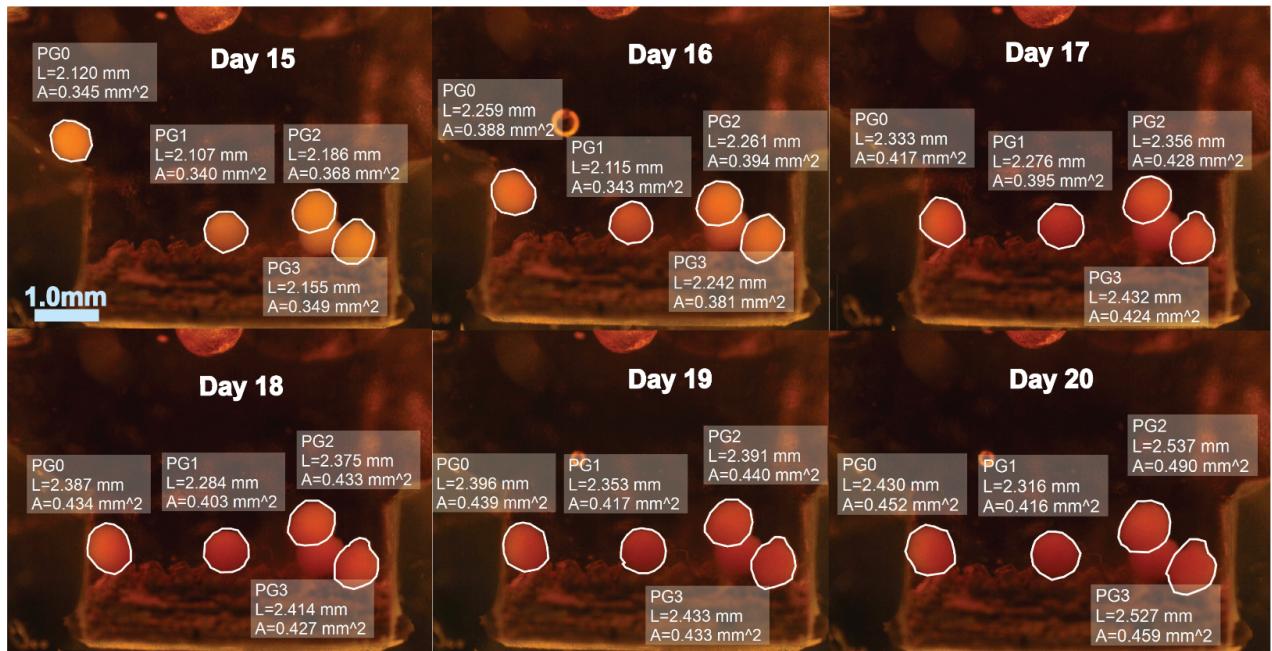

b)

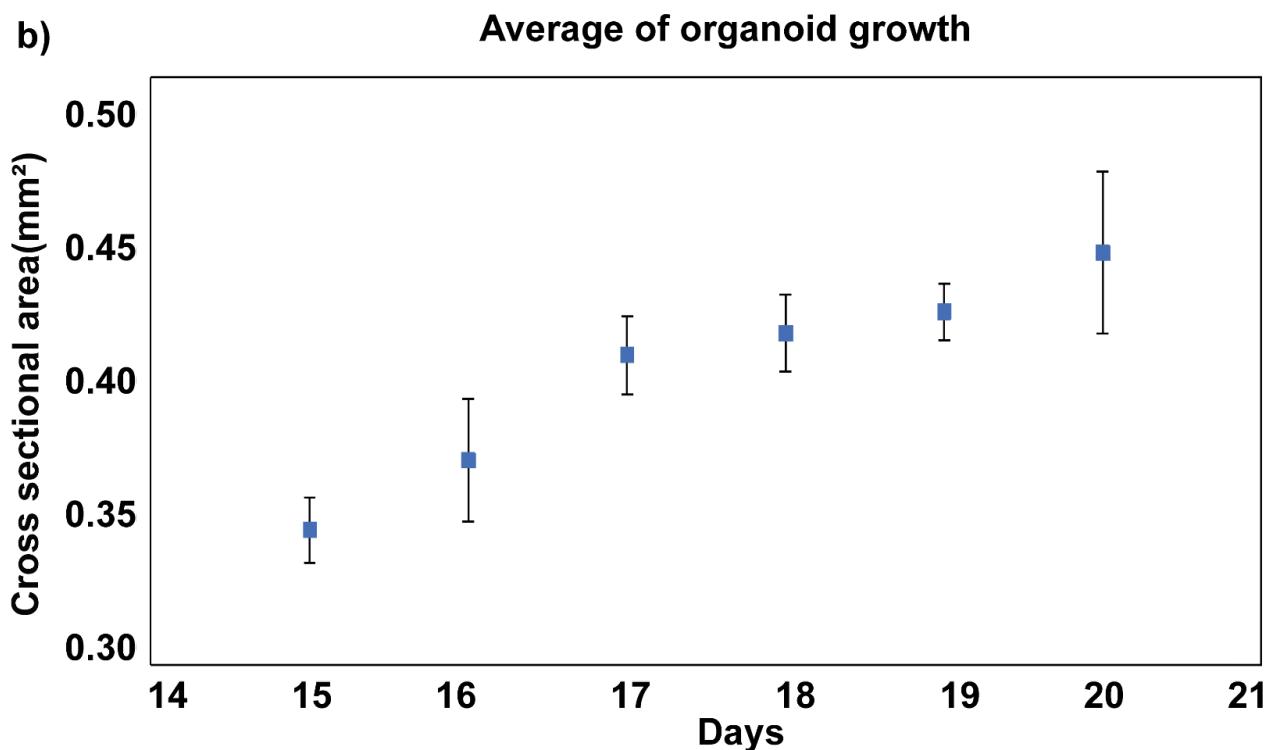


Supplementary Figure 7. Longitudinal growth of cortical organoid in batch 1. a) Estimated area. b) adjusted growth curve over 6 days.

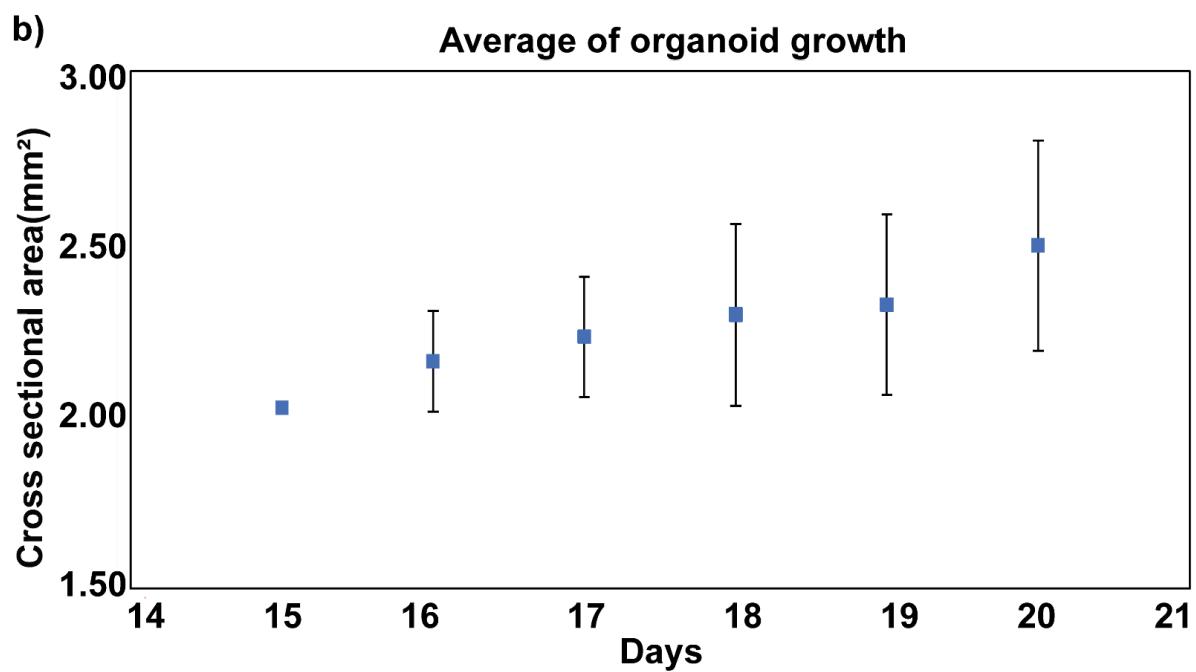


Supplementary Figure 8. Longitudinal growth of cortical organoid in batch 2. a) Estimated area. b) adjusted growth curve over 6 days.

a)

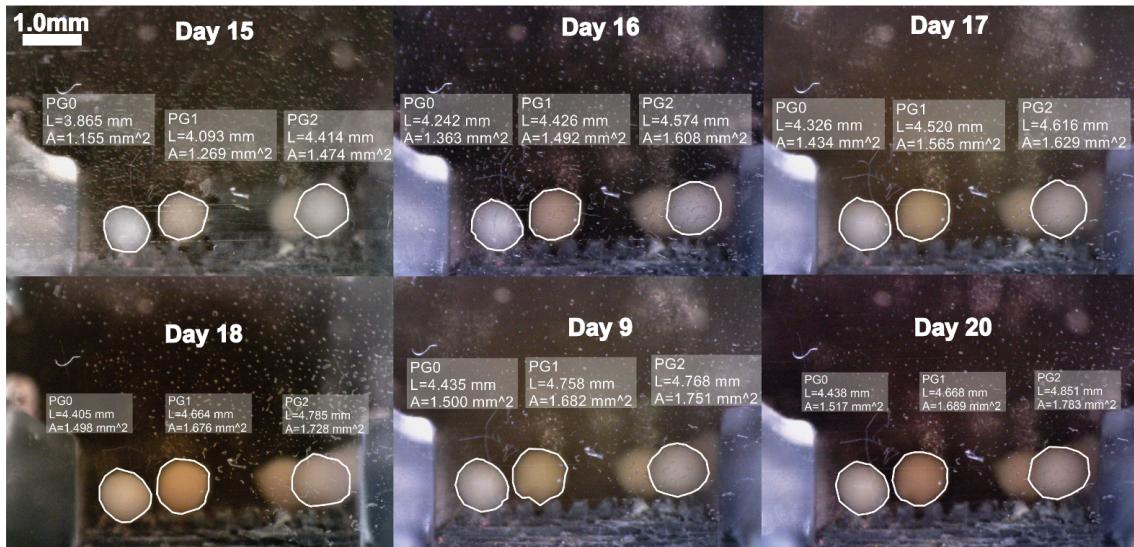

b)

### Average of organoid growth

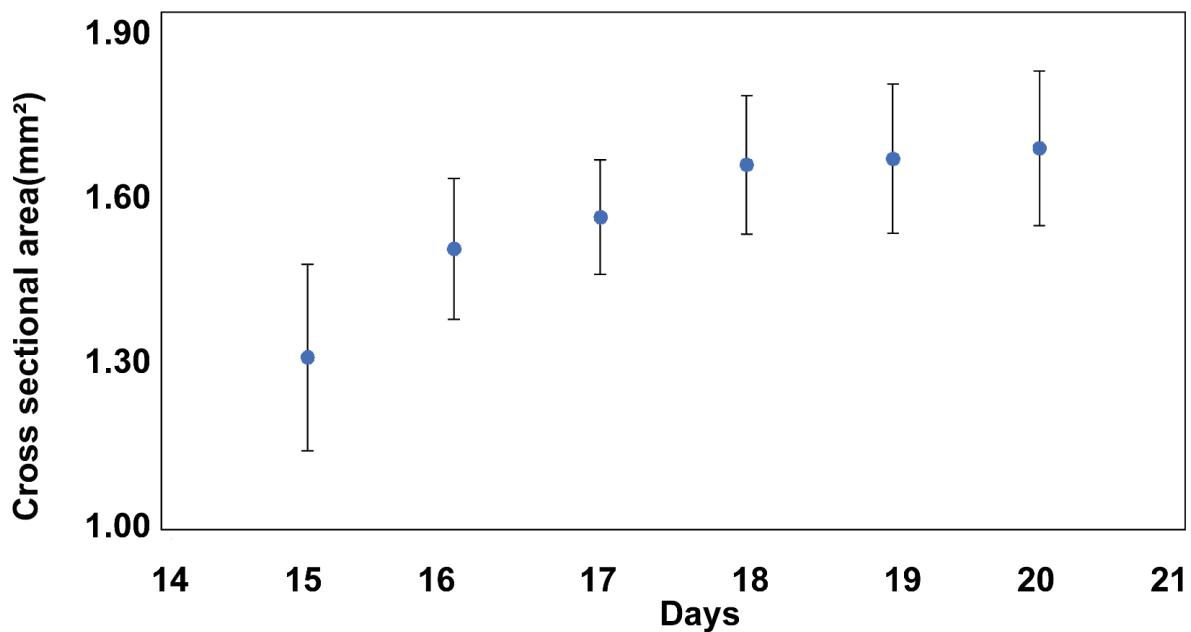

Supplementary Figure 9. Longitudinal growth of cortical organoid in batch 3. a) Estimated area. b) adjusted growth curve over 6 days.