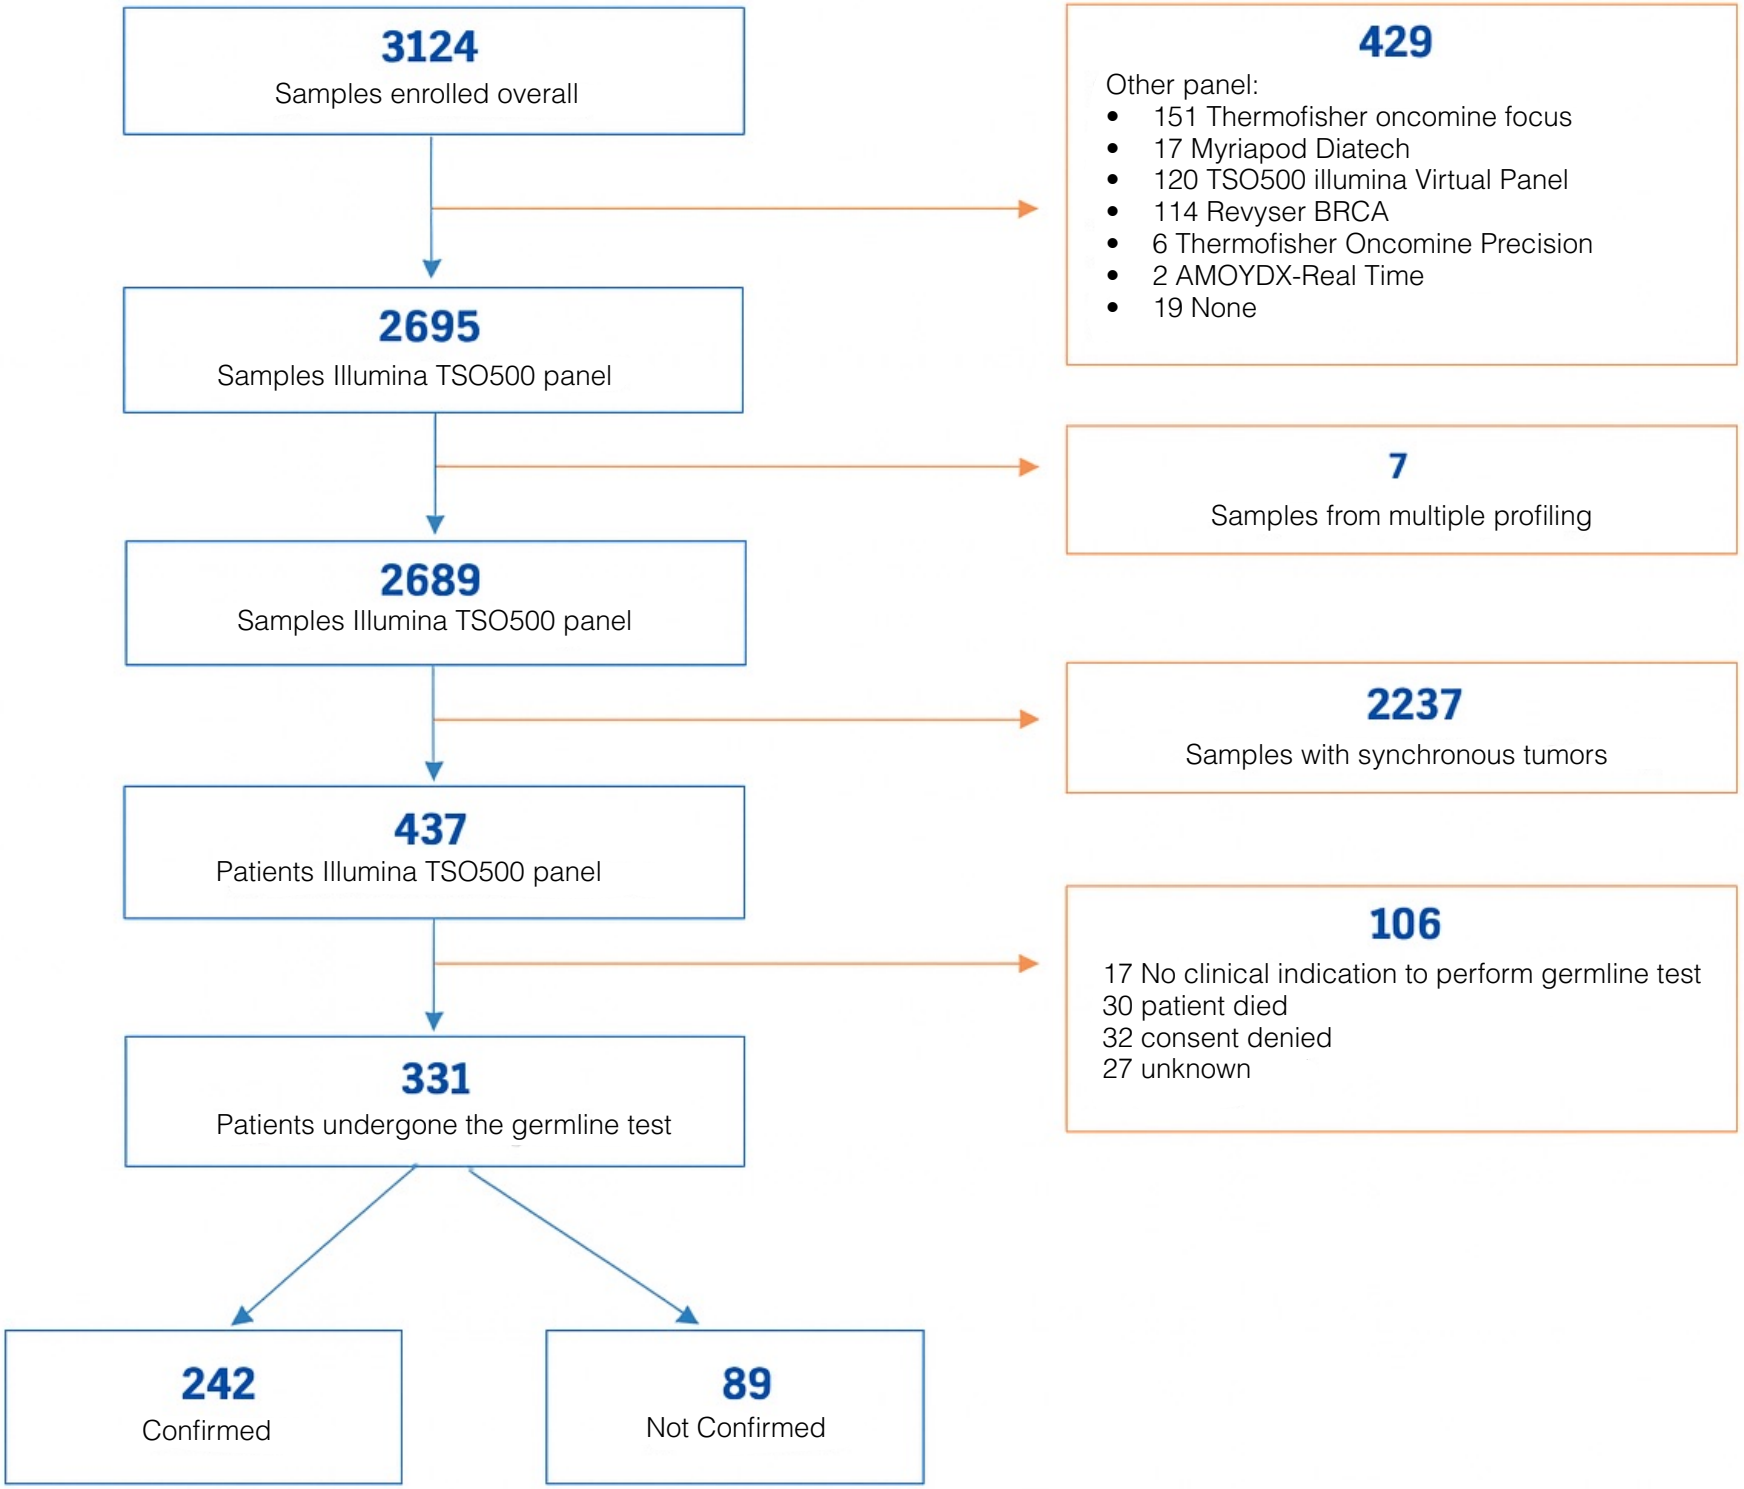
3124
Samples enrolled overall
429
Other panel:
• 151 Thermofisher oncomine focus
• 17 Myriapod Diatech
• 120 TSO500 illumina Virtual Panel
• 114 Revyser BRCA
• 6 Thermofisher Oncomine Precision
• 2 AMOYDX-Real Time
• 19 None
2695
Samples Illumina TSO500 panel
7
Samples from multiple profiling
2689
Samples Illumina TSO500 panel
2237
Samples with synchronous tumors
437
Patients Illumina TSO500 panel
106
17 No clinical indication to perform germline test
30 patient died
32 consent denied
27 unknown
331
Patients undergone the germline test
242
Confirmed
89
Not Confirmed