




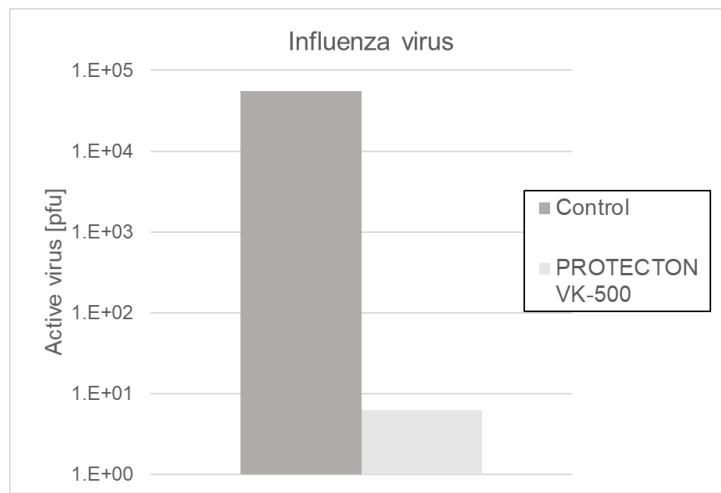


Tested by: BOKEN QUALITY EVALUATION INSTITUTE

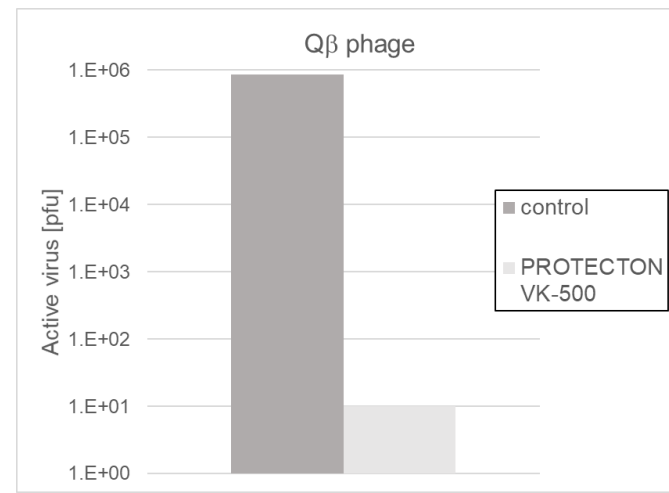

Tested by: TOTO Ltd. Research institute

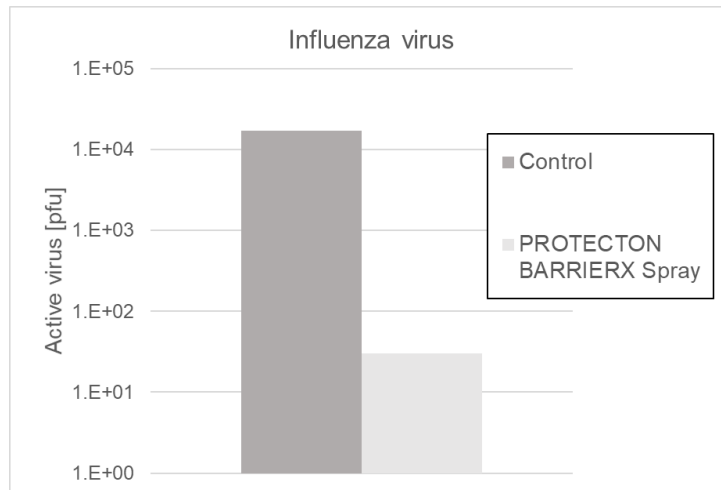

Tested by: Japan Food Research Laboratories (JFRL)

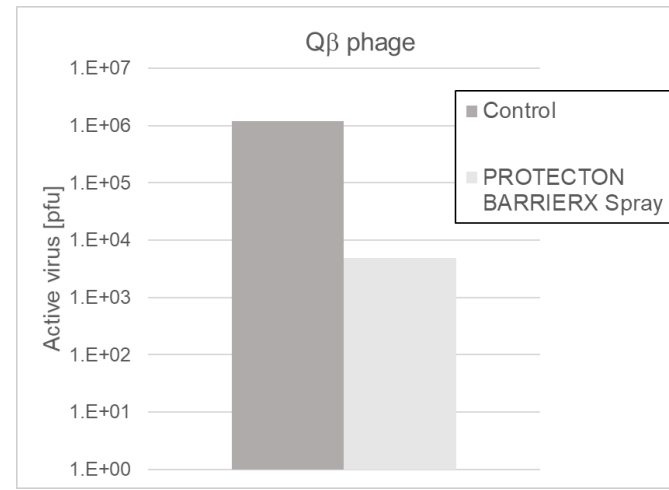

Tested by: TOTO Ltd. Research institute

Fig. S1 Validation of commercially available anti-virus products using traditional viruses.

(A, B) Effect of PROTECTON VK-500 on Influenza and Qβ phage, respectively.

(C, D) Effect of PROTECTON BARRIERX Spray on Influenza and Qβ phage, respectively.